

**IN THE UNITED STATES DISTRICT COURT
FOR THE DISTRICT OF DELAWARE**

ICU MEDICAL, INC.,)	
)	
Plaintiff,)	
)	
v.)	C.A. No. _____
)	
RYMED TECHNOLOGIES, INC.,)	
)	JURY TRIAL DEMANDED
Defendant.)	

COMPLAINT FOR PATENT INFRINGEMENT

PARTIES

1. Plaintiff ICU Medical, Inc. ("ICU") is a corporation duly organized and exhibits under the laws of the State of Delaware having a principal place of business at 951 Calle Amanecer, San Clemente, California.

2. On information and belief, Defendant RyMed Technologies, Inc. ("RyMed") is a corporation duly organized and existing under the laws of the State of Delaware, doing business in this judicial district, and having a principal place of business at 137 Third Avenue North, Franklin, Tennessee.

JURISDICTION AND VENUE

3. This is an action for damages and injunctive relief based upon patent infringement arising under Title 35 of the United States Code.

4. Upon information and belief, Defendant Rymed has transacted business in this District, contracted to supply goods or services in this District, and has otherwise purposely availed itself of the privileges and benefits of the laws of the State of Delaware. This Court has jurisdiction over RyMed because RyMed is a Delaware corporation and also because it has committed acts of patent infringement during the course of its business in this District.

5. This Court has jurisdiction over the subject matter of this action pursuant to 28 U.S.C. § 1331 and 28 U.S.C. § 1338.

6. Venue is proper in this District pursuant to 28 U.S.C. §§ 1400(b) and 1391.

THE PATENTS IN SUIT

7. On November 11, 1997, United States Patent No. 5,865,866 (“the ’866 patent”) entitled “Medical valve and method of use” was duly and legally issued to ICU. ICU is the owner of the entire right, title, and interest in the and to the ’866 patent. A true and correct copy of the ’866 patent is attached hereto as Exhibit A to this Complaint.

8. On February 23, 1999, United States Patent No. 5,873,862 (“the ’862 patent”) entitled “Medical valve and method of use” was duly and legally issued to ICU. ICU is the owner of the entire right, title, and interest in and to the ’862 patent. A true and correct copy of the ’862 patent is attached hereto as Exhibit B to this Complaint.

9. On July 27, 1999, United States Patent No. 5,928,204 (“the ’204 patent”) entitled “Medical valve and method of use” was duly and legally issued to ICU. ICU is the owner of the entire right, title, and interest in and to the ’204 patent. A true and correct copy of the ’204 patent is attached hereto as Exhibit C to this Complaint.

10. On June 3, 2003, United States Patent No. 6,572,592 (“the ’592 patent”) entitled “Medical valve and method of use” was duly and legally issued to ICU. ICU is the owner of the entire right, title, and interest in the and to the ’592 patent. A true and correct copy of the ’592 patent is attached hereto as Exhibit D to this Complaint.

COUNT I

DIRECT INFRINGEMENT OF THE '866 PATENT

11. ICU realleges and incorporates herein by reference the allegations contained in paragraphs 1-10.

12. On information and belief, RyMed has infringed and continues to infringe, literally or under the doctrine of equivalents, one or more claims of the '866 patent. RyMed's infringing activities in the United States and this District include the development, manufacture, use, importation, sale, and/or offer for sale of products, including but not limited to its InVision-Plus valve. Such products have no substantial non-infringing use. RyMed's infringing activities violate 35 U.S.C. § 271.

13. On information and belief, RyMed's infringement has been, and continues to be, willful and deliberate, and has caused substantial damage to ICU.

14. On information and belief, RyMed's infringement in violation of the federal patents laws will continue to injure ICU unless otherwise enjoined by this Court.

COUNT II

**DIRECT, INDUCED, AND/OR CONTRIBUTORY INFRINGEMENT
OF THE '862 PATENT**

15. ICU realleges and incorporates herein by reference the allegations contained in paragraphs 1-14.

16. On information and belief, RyMed has infringed and continues to infringe has induced and continues to induce others to infringe; and/or has committed and continues to commit acts of contributory infringement, literally or under the doctrine of equivalents, of one or more claims of the '862 patent. RyMed's infringing activities in the United States and this District include the development, manufacture, use, importation, sale, and/or offer for sale of

products, including but not limited to its InVision-Plus valve, and inducing others to do the same. Such products have no substantial non-infringing use. RyMed's infringing activities violate 35 U.S.C. § 271.

17. On information and belief, RyMed's direct, induced, and/or contributory infringement has been, and continues to be, willful and deliberate, and has caused substantial damage to ICU.

18. On information and belief, RyMed's infringement in violation of the federal patents laws will continue to injure ICU unless otherwise enjoined by this Court.

COUNT III

DIRECT INFRINGEMENT OF THE '204 PATENT

19. ICU realleges and incorporates herein by reference the allegations contained in paragraphs 1-18.

20. On information and belief, RyMed has infringed and continues to infringe, literally or under the doctrine of equivalents, one or more claims of the '204 patent. RyMed's infringing activities in the United States and this District include the development, manufacture, use, importation, sale, and/or offer for sale of products, including but not limited to its InVision-Plus valve. Such products have no substantial non-infringing use. RyMed's infringing activities violate 35 U.S.C. § 271.

21. On information and belief, RyMed's direct infringement has been, and continues to be, willful and deliberate, and has caused substantial damage to ICU.

22. On information and belief, RyMed's direct infringement in violation of the federal patents laws will continue to injure ICU unless otherwise enjoined by this Court.

COUNT IV

**DIRECT, INDUCED, AND/OR CONTRIBUTORY INFRINGEMENT
OF THE '592 PATENT**

23. ICU realleges and incorporates herein by reference the allegations contained in paragraphs 1-22.

24. On information and belief, RyMed has infringed and continues to infringe; has induced and continues to induce others to infringe; and/or has committed and continues to commit acts of contributory infringement, literally or under the doctrine of equivalents, of one or more claims of the '592 patent. RyMed's infringing activities in the United States and this District include the development, manufacture, use, importation, sale, and/or offer for sale of products, including but not limited to its InVision-Plus valve, and inducing others to do the same. Such products have no substantial non-infringing use. RyMed's infringing activities violate 35 U.S.C. § 271.

25. On information and belief, RyMed's direct, induced, and/or contributory infringement has been, and continues to be, willful and deliberate, and has caused substantial damage to ICU.

26. On information and belief, RyMed's infringement in violation of the federal patents laws will continue to injure ICU unless otherwise enjoined by this Court.

PRAYER FOR RELIEF

WHEREFORE, Plaintiff prays for judgment and relief as follows:

1. A judgment that RyMed has directly infringed the '866 patent, literally or under the doctrine of equivalents, in violation of 35 U.S.C. § 271.

2. A judgment that RyMed has infringed, induced infringement of, and/or contributorily infringed, literally or under the doctrine of equivalents, the '862 patent in violation of 35 U.S.C. § 271.

3. A judgment that RyMed has infringed, literally or under the doctrine of equivalents, the '204 patent in violation of 35 U.S.C. § 271.

4. A judgment that RyMed has infringed, induced infringement of, and/or contributorily infringed, literally or under the doctrine of equivalents, the '592 patent in violation of 35 U.S.C. § 271.

5. Preliminary and permanent injunctive relief enjoining defendant RyMed, its officers, agents, servants, employees, attorneys, and all other person in active concert or participation with them as follows:

a. from selling or offering to sell any product falling within the scope of the claims of the '866, '862, '204, and '592 patents;

b. from importing any product into the United States falling within the scope of the claims of the '866, '862, '204, and '592 patents;

c. from using any product or method falling within the scope of the claims of the '866, '862, '204, and '592 patents;

d. from actively inducing others to infringe any claims of the '862, and '592 patents;

e. from engaging in acts constituting contributory infringement of any of the claims of the '862 and '592 patents;

f. from all other acts of infringement of any of the claims of the '866, '862, '204, and '592 patents;

6. A declaration that RyMed's infringement of the '866, '862, '204, and '592 patents was willful and deliberate and that this case is exceptional pursuant to 35 U.S.C. §§ 284 and 285;
7. An award of damages adequate to compensate ICU for RyMed's infringement of the '866, '862, '204, and '592 patents;
8. An award of treble damages resulting from RyMed's willful and deliberate infringement, and all other categories of damages allowed by 35 U.S.C. § 284;
9. An award of ICU's costs, expenses, and attorneys' fee incurred in bringing and prosecuting this action, including pursuant to 35 U.S.C. § 285;
10. An award of pre-judgment interest; and
11. For such further relief as this Court deems ICU may be entitled to in law and in equity.


JURY DEMAND

ICU demands a jury trial on all issues triable to a jury in this matter.

POTTER ANDERSON & CORROON LLP

OF COUNSEL:

James Pooley
Marc Peters
Kimberly Van Voorhis
MORRISON & FOERSTER, LLP
755 Page Mill Rd.
Palo Alto, CA 94304
Tel: (650) 813-5600

By: 
Richard L. Horwitz (#2246)
Kenneth L. Dorsney (#3726)
Hercules Plaza, 6th Floor
1313 N. Market Street
Wilmington, DE 19899
Tel: (302) 984-6000
rhorwitz@potteranderson.com
kdorsney@potteranderson.com

Dated: July 27, 2007
809486 / 32116

Attorneys for Plaintiff ICU Medical, Inc.

EXHIBIT A



US005685866A

United States Patent [19]

Lopez

[11] Patent Number: 5,685,866

[45] Date of Patent: Nov. 11, 1997

[54] MEDICAL VALVE AND METHOD OF USE

[75] Inventor: George A. Lopez, Corona del Mar, Calif.

[73] Assignee: ICU Medical, Inc., San Clemente, Calif.

[21] Appl. No.: 334,846

[22] Filed: Nov. 4, 1994

Related U.S. Application Data

[63] Continuation of Ser. No. 96,659, Jul. 23, 1993, which is a continuation-in-part of PCT/US92/10367, Dec. 1, 1992, which is a continuation-in-part of Ser. No. 813,073, Dec. 18, 1991, abandoned.

[51] Int. Cl.⁶ A61M 5/00

[52] U.S. Cl. 604/249; 604/256

[58] Field of Search 604/246, 249, 604/247, 256, 283

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 321,250 10/1991 Jepson et al. .
 D. 321,251 10/1991 Jepson et al. .
 1,578,517 3/1926 Hein .
 2,289,677 7/1942 Perelson .
 2,847,995 8/1958 Adams .
 3,134,380 5/1964 Armao .
 3,354,881 11/1967 Bloch .
 3,648,684 3/1972 Barnwell et al. .
 3,852,385 12/1974 Huggins .
 3,974,832 8/1976 Kruck .
 3,976,063 8/1976 Henneman et al. .
 3,986,508 10/1976 Barrington .
 4,019,512 4/1977 Tenczar .
 4,076,285 2/1978 Martinez .
 4,080,965 3/1978 Phillips .
 4,121,585 10/1978 Becker, Jr. .
 4,128,098 12/1978 Bloom et al. .
 4,161,949 7/1979 Thanawalla .
 4,187,846 2/1980 Lolachi et al. .
 4,219,912 9/1980 Adams .
 4,328,802 5/1982 Curley et al. .

- 4,334,551 6/1982 Pfister .
 4,338,933 7/1982 Bayard et al. .
 4,411,662 10/1983 Pearson .
 4,432,759 2/1984 Gross et al. .
 4,432,765 2/1984 Oscarsson .
 4,439,193 3/1984 Larkin .
 4,457,749 7/1984 Bellotti et al. .
 4,508,367 4/1985 Oreopoulos et al. .

(List continued on next page.)

FOREIGN PATENT DOCUMENTS


- 1 105 959 7/1981 Canada .
 0 114 677 A2 8/1984 European Pat. Off. .
 0 237 321 10/1987 European Pat. Off. .
 0 240 987 A2 10/1987 European Pat. Off. .
 0 309 771 A1 9/1988 European Pat. Off. .
 0 446 463 A1 12/1990 European Pat. Off. .
 84 25 197 U 9/1985 Germany .
 WO 86/01712 3/1986 WIPO .
 WO 86/03416 6/1986 WIPO .
 WO 93/11828 6/1993 WIPO .

Primary Examiner—Corrine M. McDermott
 Attorney, Agent, or Firm—Knobbe, Martens, Olson & Bear, LLP

[57] ABSTRACT

A closed system, needleless valve device includes a generally tubular body defining an internal cavity. On the proximal end of the body there is an opening which is preferably sufficiently large to receive an ANSI standard tip of a medical implement. The distal end of the body has a generally tubular skirt. The valve also includes a hollow spike having a closed tip. The spike includes at least one longitudinal 18-gauge hole located distal the tip, and is seated inside the cavity such that the tip is below the proximal end of the body. An annular support cuff is connected to the spike which seals off a portion of the cavity of the body such that an upper cavity containing the tip is defined. The valve also includes a plastic, resilient silicone seal which fills the upper cavity and opening and covers the tip of the spike so as to present a flush surface. An adaptor enables the valve to be attached to a resealable container.

17 Claims, 19 Drawing Sheets

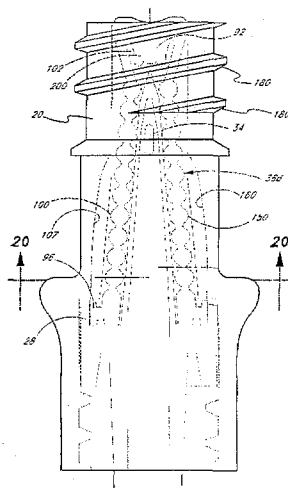

5,685,866

Page 2

U.S. PATENT DOCUMENTS

4,511,359	4/1985	Vaillancourt .	4,981,469	1/1991	Whitehouse et al. .
4,512,766	4/1985	Vaillancourt .	4,998,713	3/1991	Vaillancourt .
4,592,356	6/1986	Gutierrez .	4,998,921	3/1991	Vickroy et al. .
4,610,469	9/1986	Wolff-Mooij 285/260	4,998,927	3/1991	Vaillancourt .
4,617,012	10/1986	Vaillancourt .	5,069,225	12/1991	Okamura .
4,645,494	2/1987	Lee et al. .	5,100,394	3/1992	Dudar et al. .
4,673,400	6/1987	Martin .	5,122,123	6/1992	Vaillancourt .
4,706,487	11/1987	Bandou et al. .	5,134,489	7/1992	Jepson et al. .
4,725,267	2/1988	Vaillancourt .	5,154,703	10/1992	Bonaldo .
4,752,292	6/1988	Lopez et al. .	5,158,554	10/1992	Jepson et al. .
4,775,369	10/1988	Schwartz .	5,167,642	12/1992	Fowles .
4,781,702	11/1988	Herli .	5,167,648	12/1992	Jepson et al. .
4,810,241	3/1989	Rogers .	5,171,234	12/1992	Jepson et al. .
4,846,809	7/1989	Sims .	5,188,620	2/1993	Jepson et al. .
4,874,377	10/1989	Newgard et al. .	5,273,533	12/1993	Bonaldo .
4,950,260	8/1990	Bonaldo .	5,290,254	3/1994	Vaillancourt .
4,964,855	10/1990	Todd et al. .	5,344,414	9/1994	Lopez .
4,969,883	11/1990	Gilbert et al. .	5,401,245	3/1995	Haining .

U.S. Patent

Nov. 11, 1997

Sheet 1 of 19

5,685,866

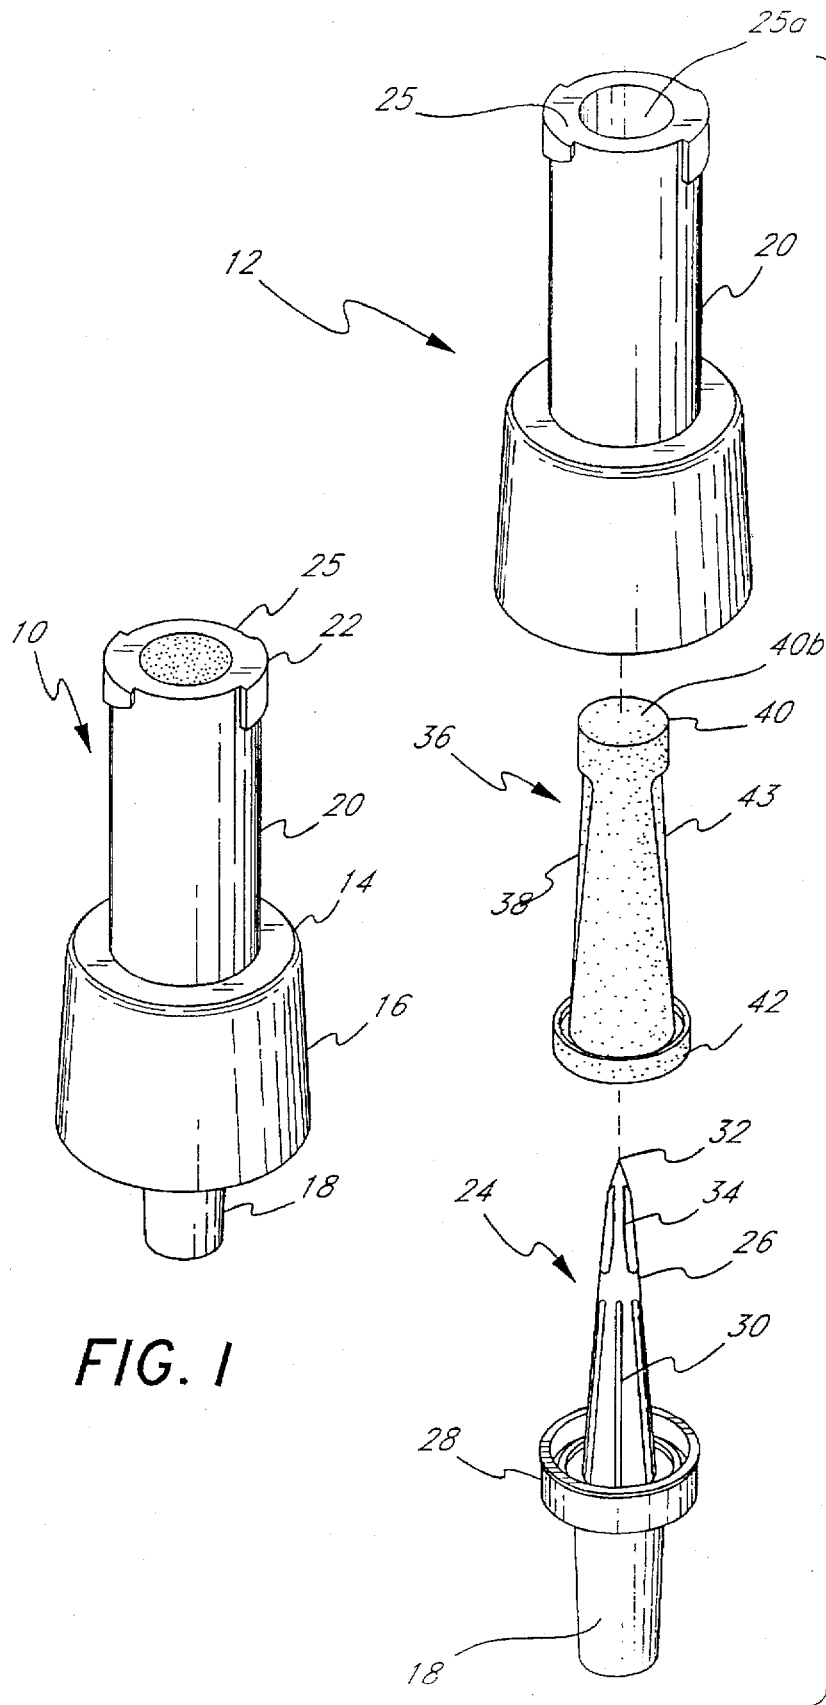


FIG. 1

FIG. 2

U.S. Patent

Nov. 11, 1997

Sheet 2 of 19

5,685,866

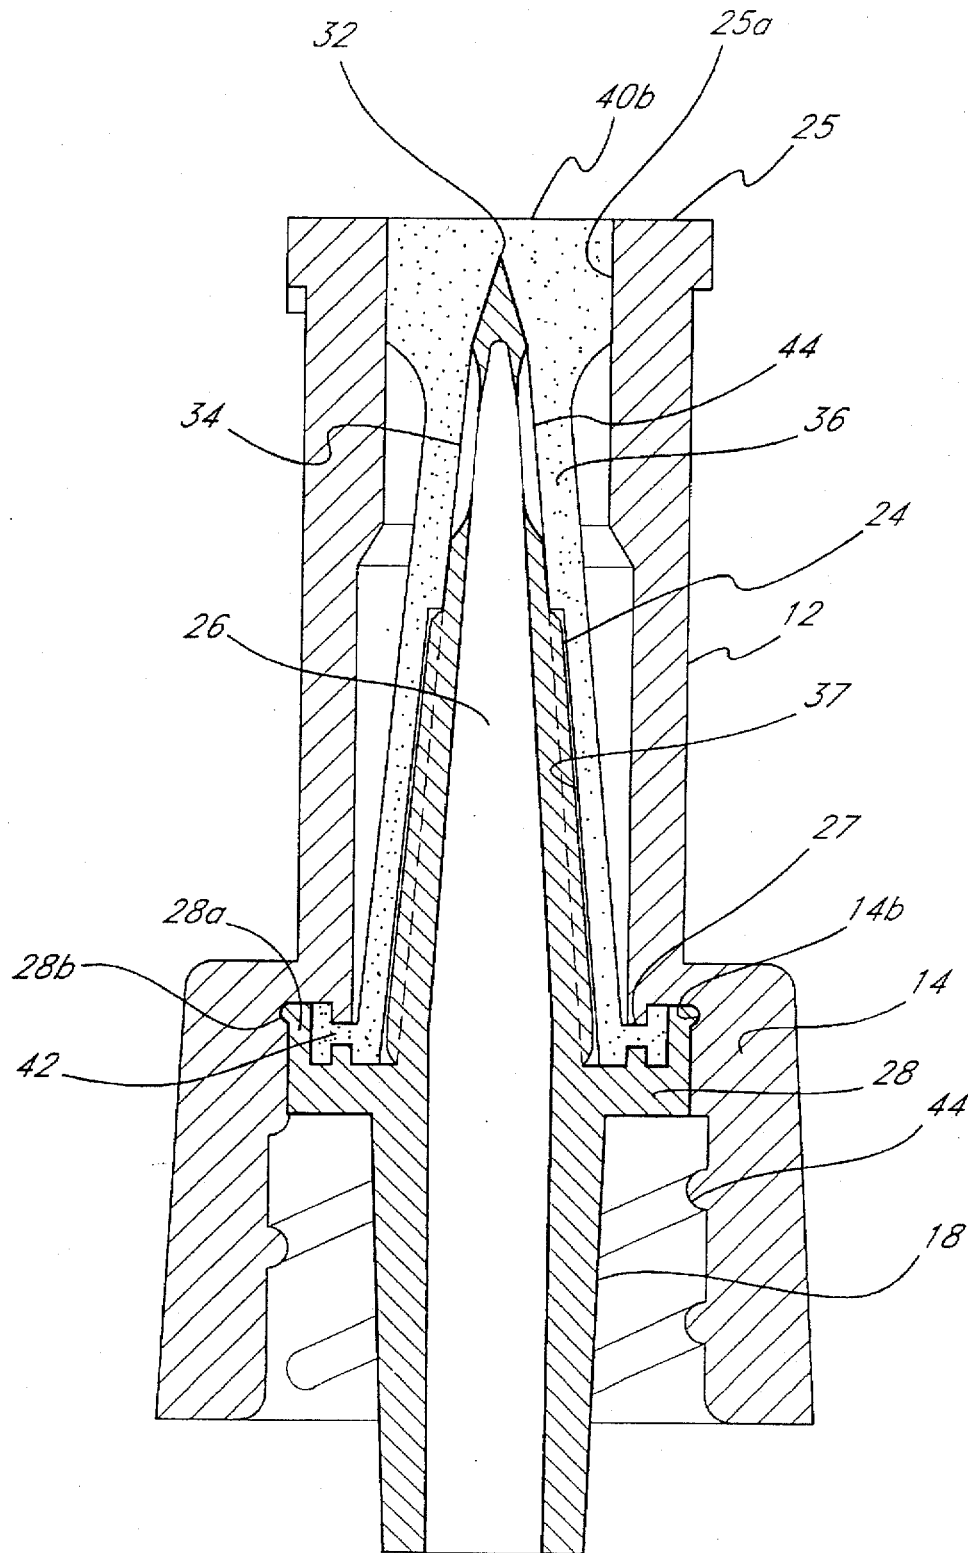


FIG. 3

U.S. Patent

Nov. 11, 1997

Sheet 3 of 19

5,685,866

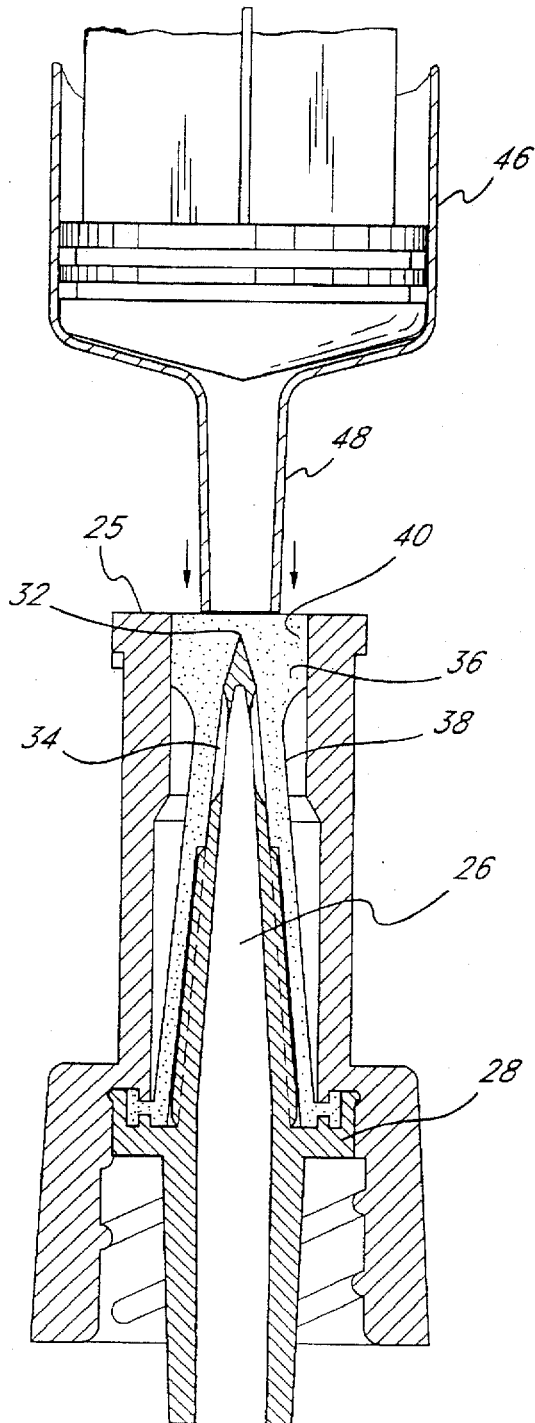


FIG. 4

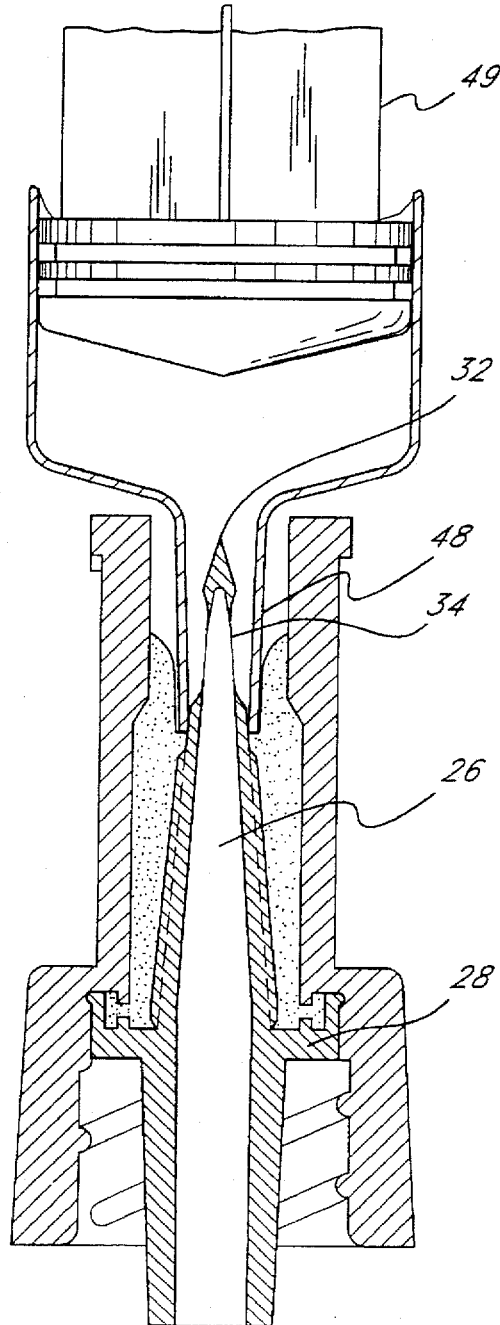


FIG. 5

FIG. 6

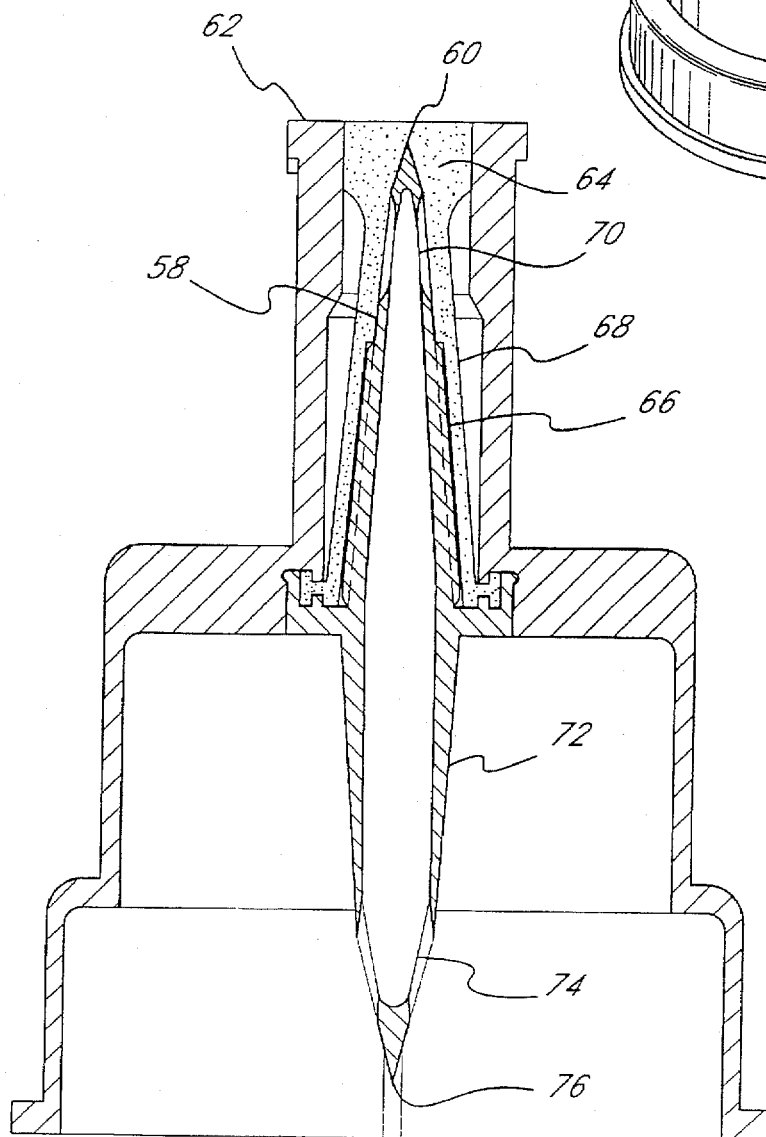
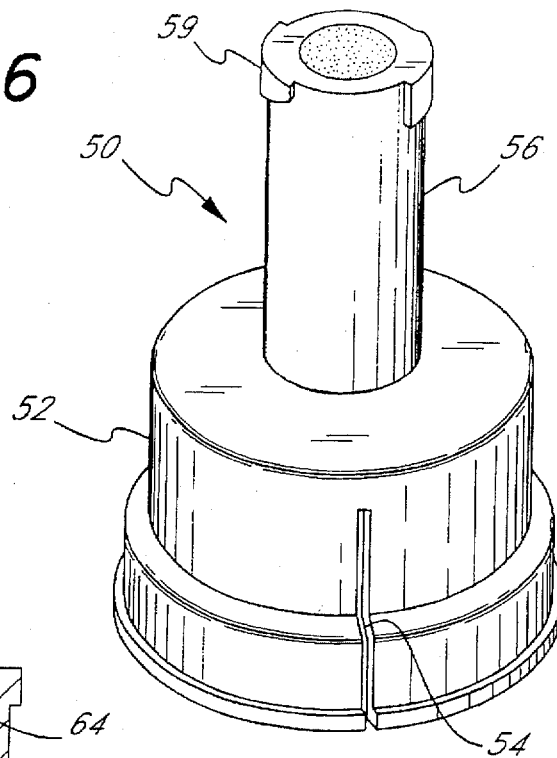


FIG. 7


U.S. Patent

Nov. 11, 1997

Sheet 5 of 19

5,685,866

FIG. 8

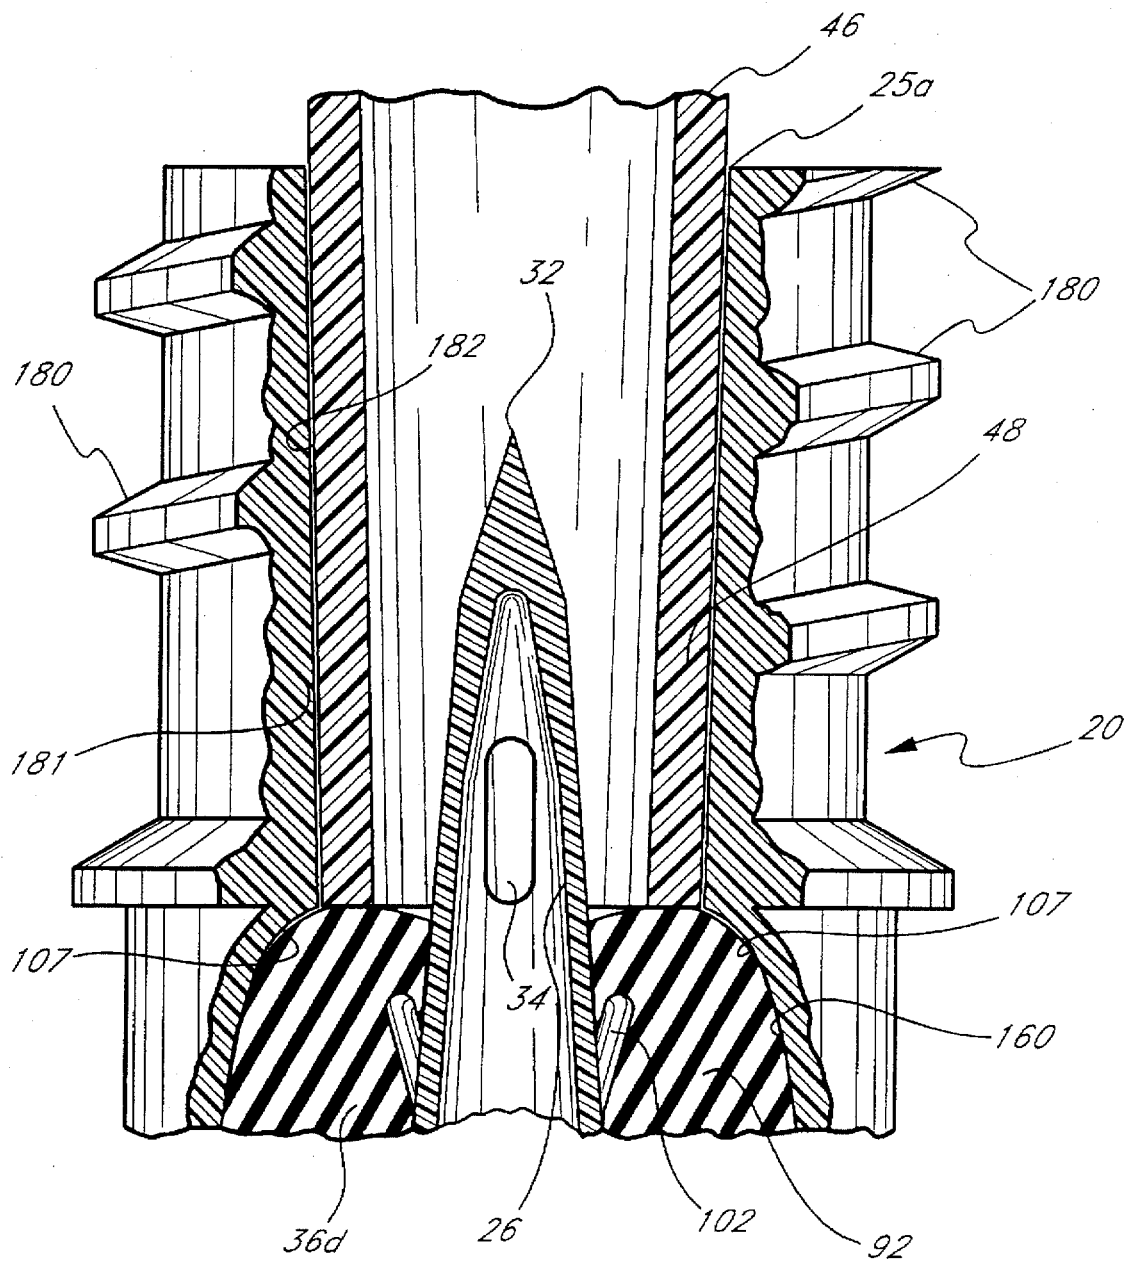

U.S. Patent

Nov. 11, 1997

Sheet 6 of 19

5,685,866

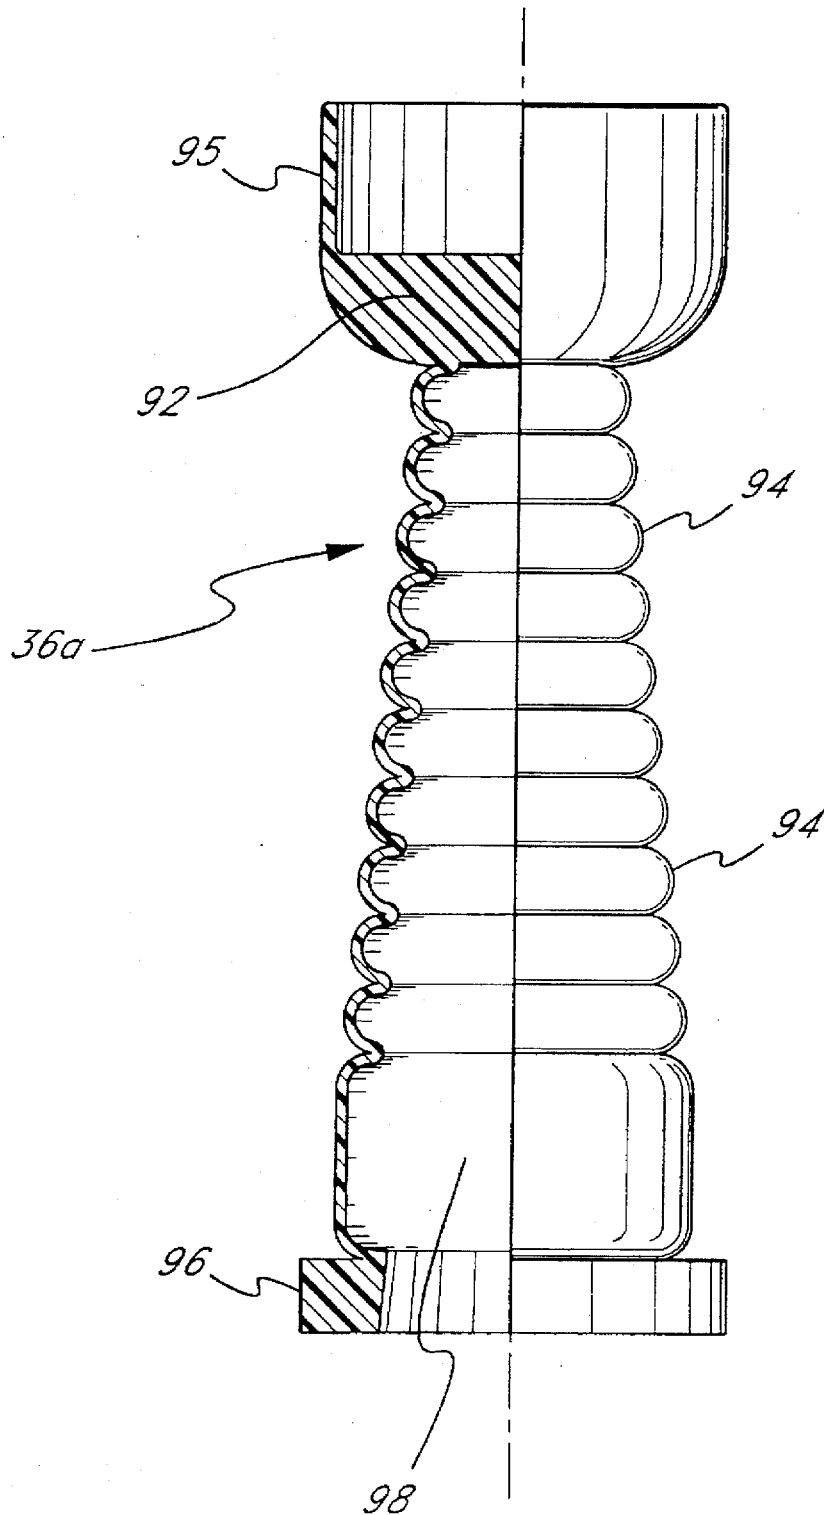


FIG. 9

U.S. Patent

Nov. 11, 1997

Sheet 8 of 19

5,685,866

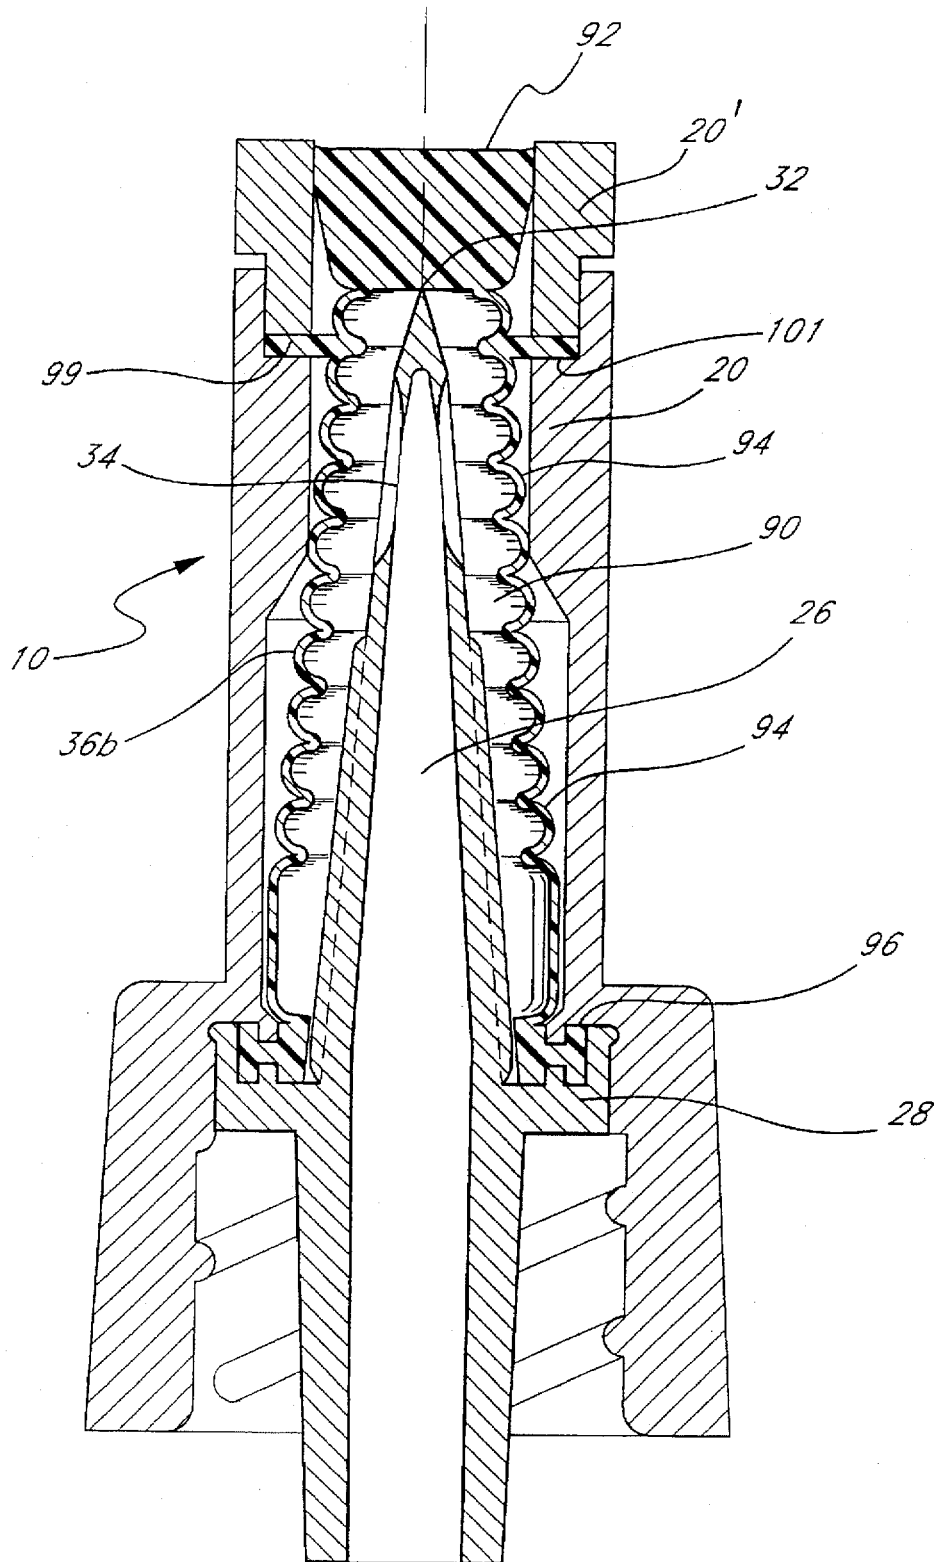


FIG. 11

U.S. Patent

Nov. 11, 1997

Sheet 10 of 19

5,685,866

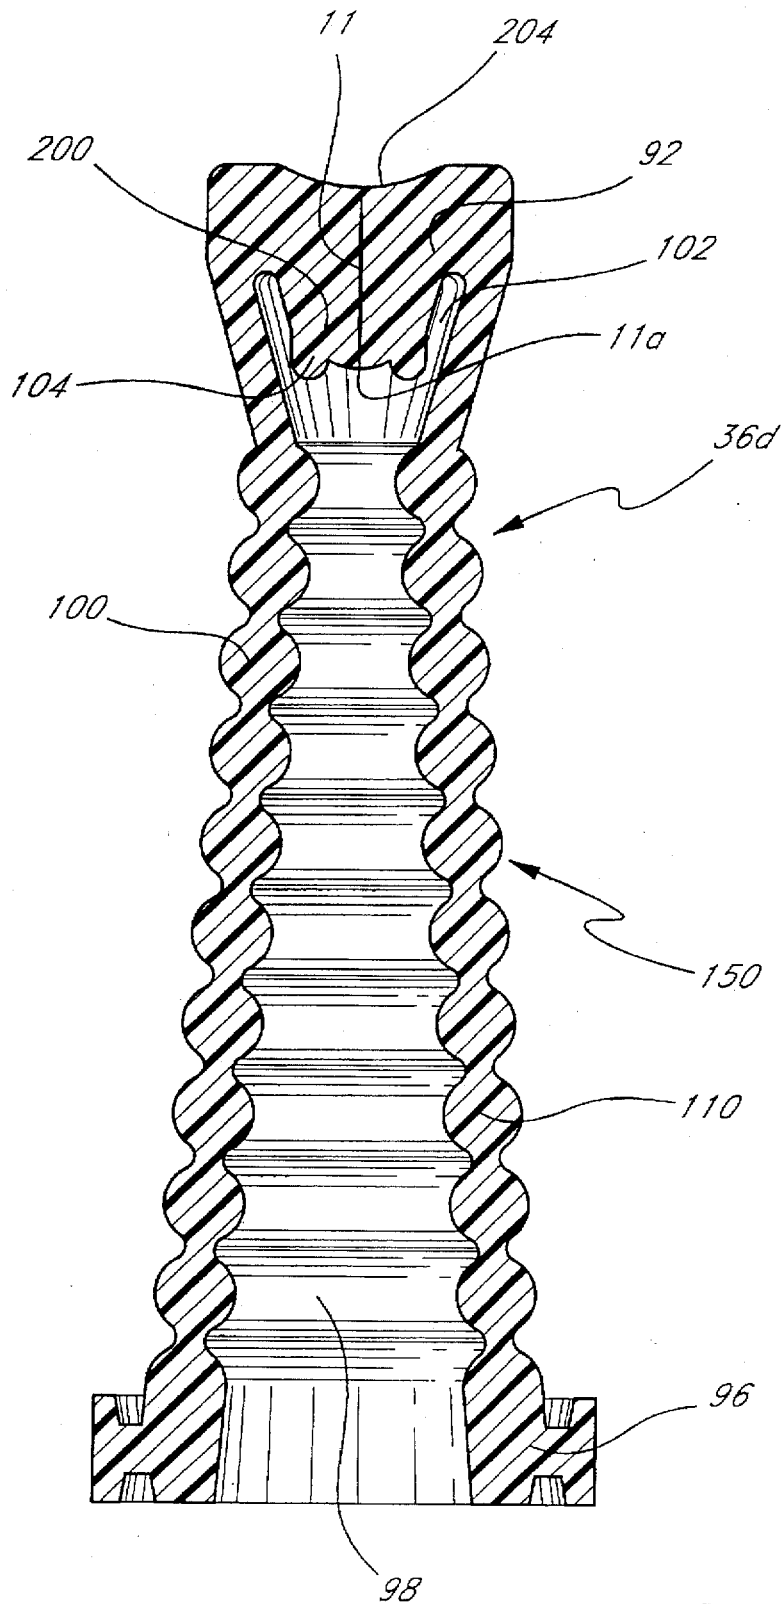


FIG. 13

U.S. Patent

Nov. 11, 1997

Sheet 11 of 19

5,685,866

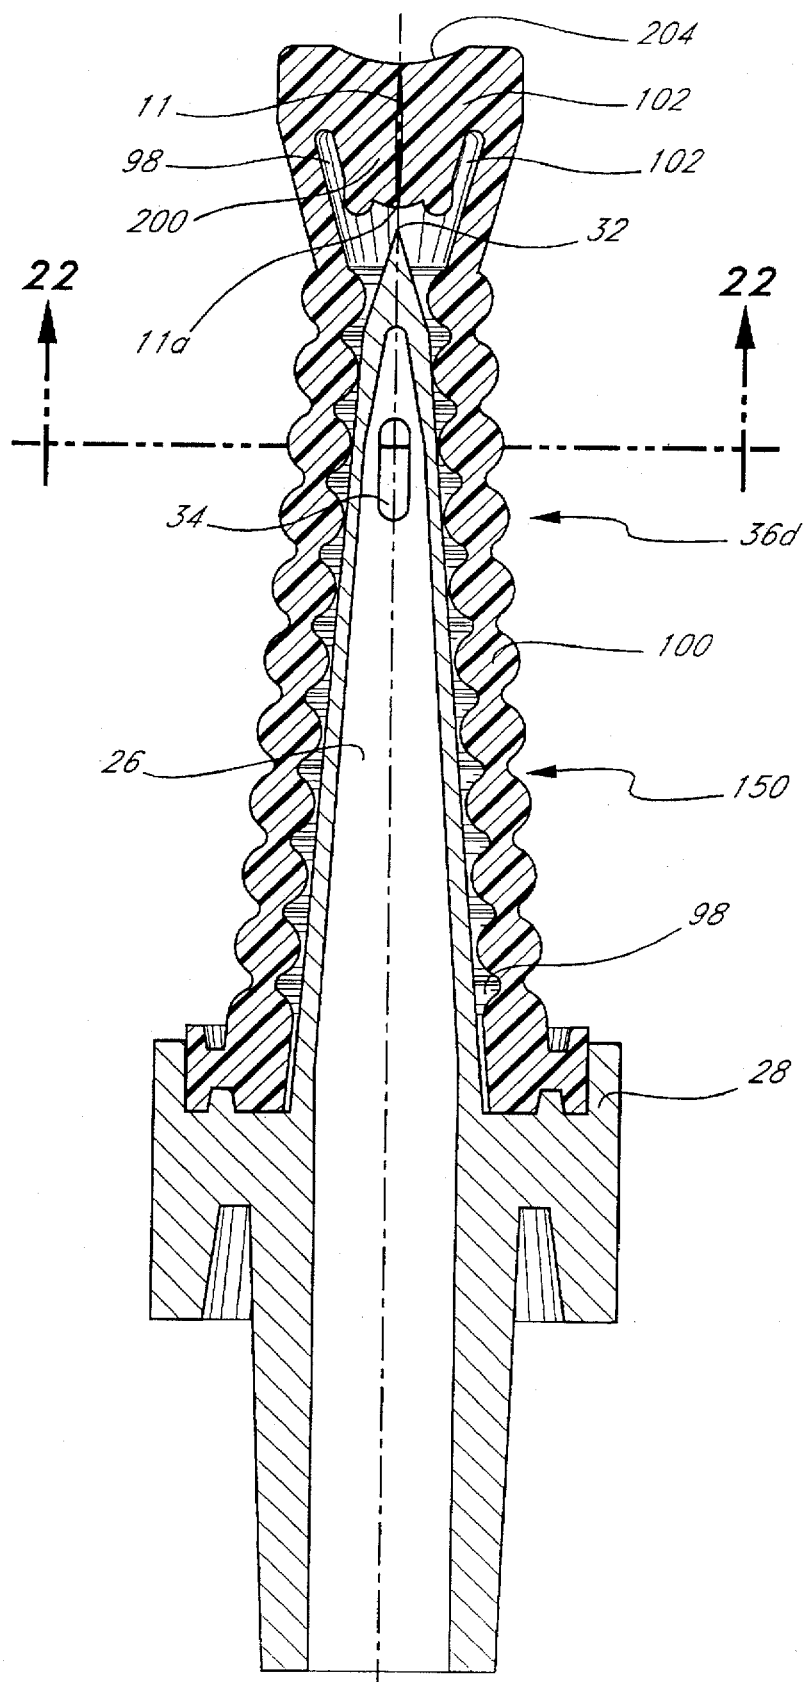


FIG. 14

U.S. Patent

Nov. 11, 1997

Sheet 12 of 19

5,685,866

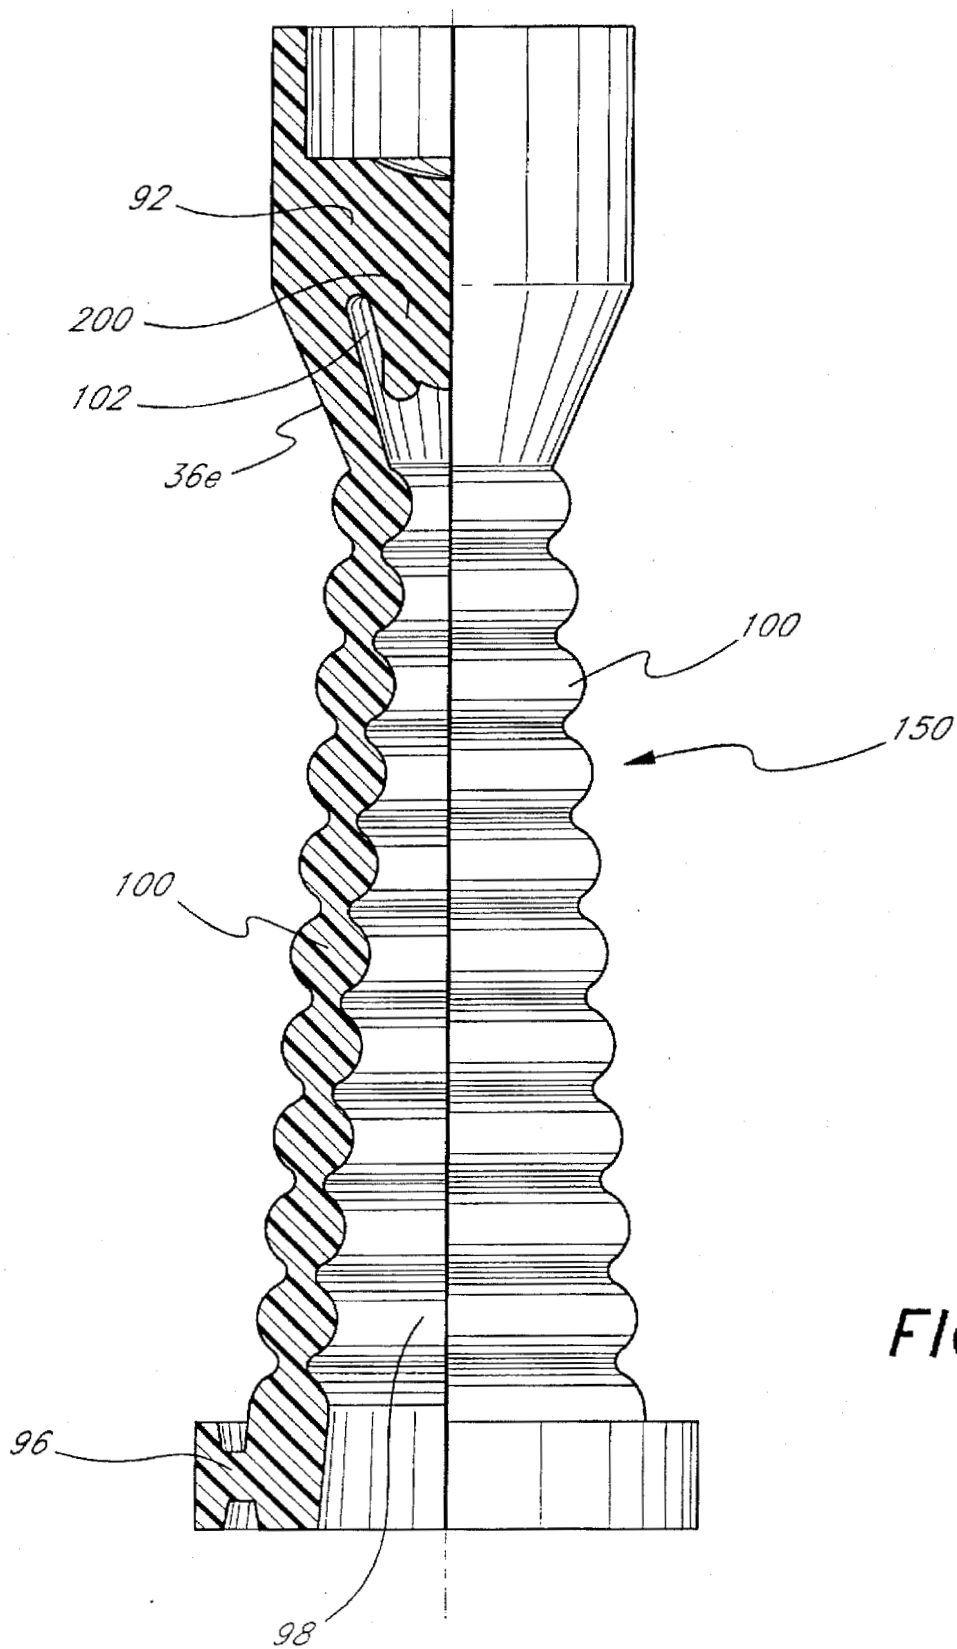


FIG. 15

U.S. Patent

Nov. 11, 1997

Sheet 13 of 19

5,685,866

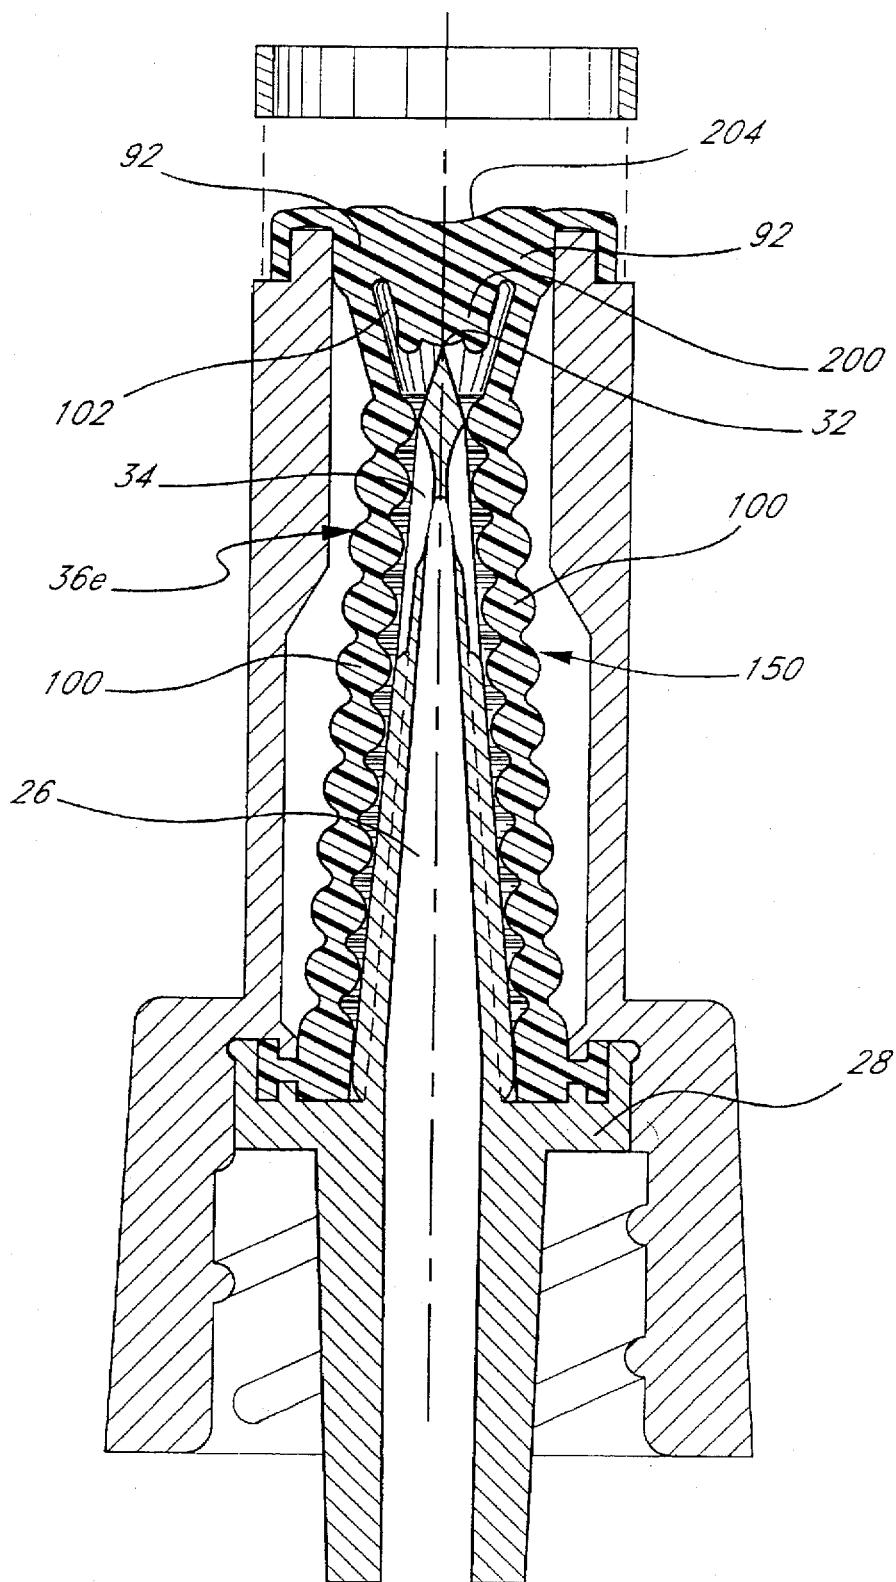


FIG. 16

U.S. Patent

Nov. 11, 1997

Sheet 15 of 19

5,685,866


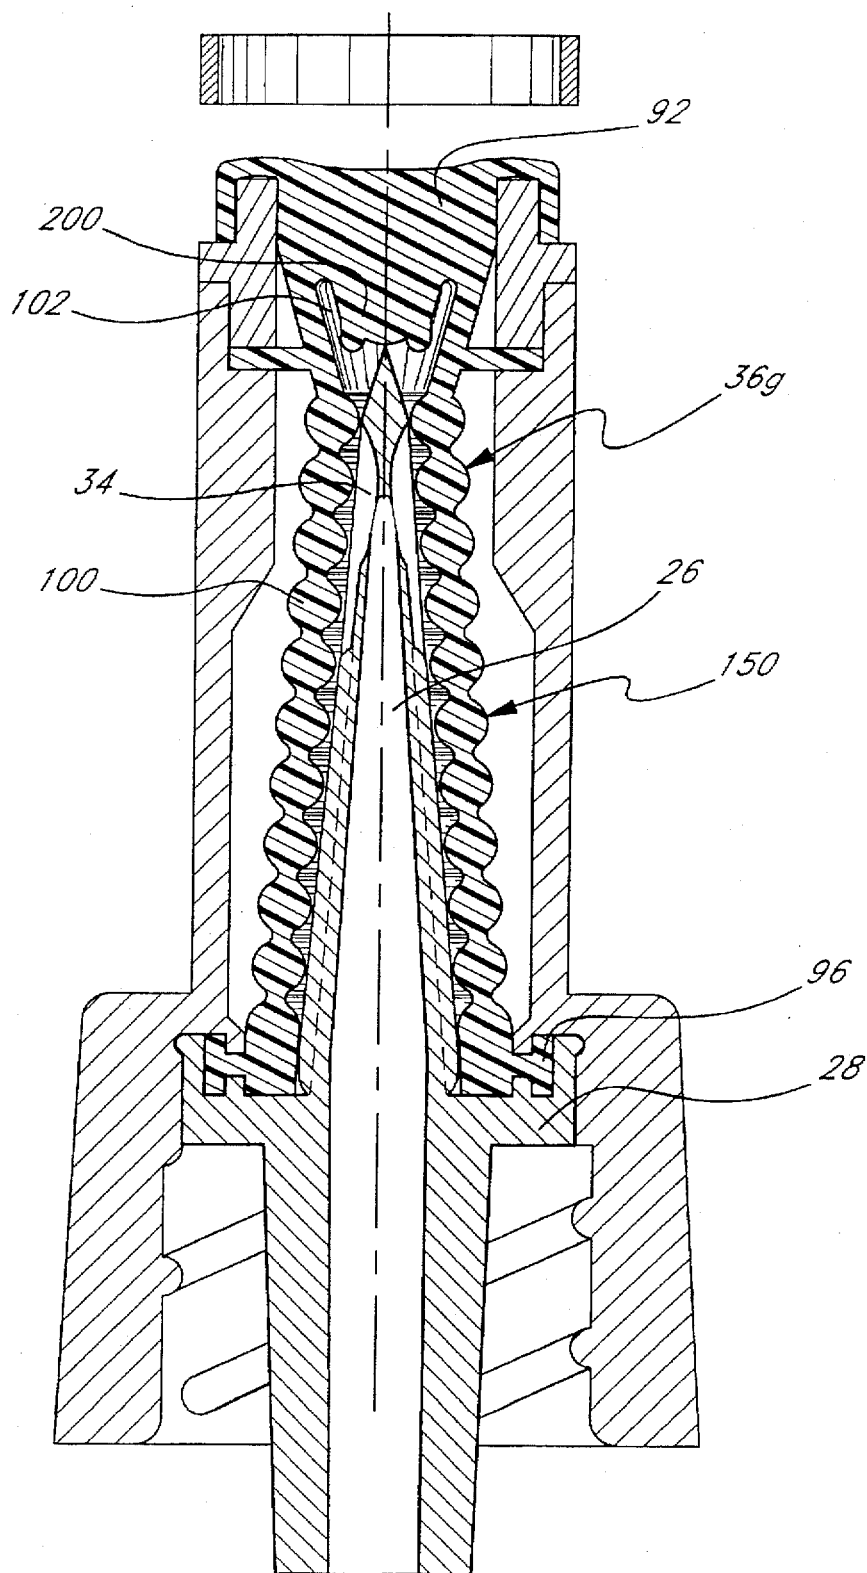


FIG. 18

FIG. 19

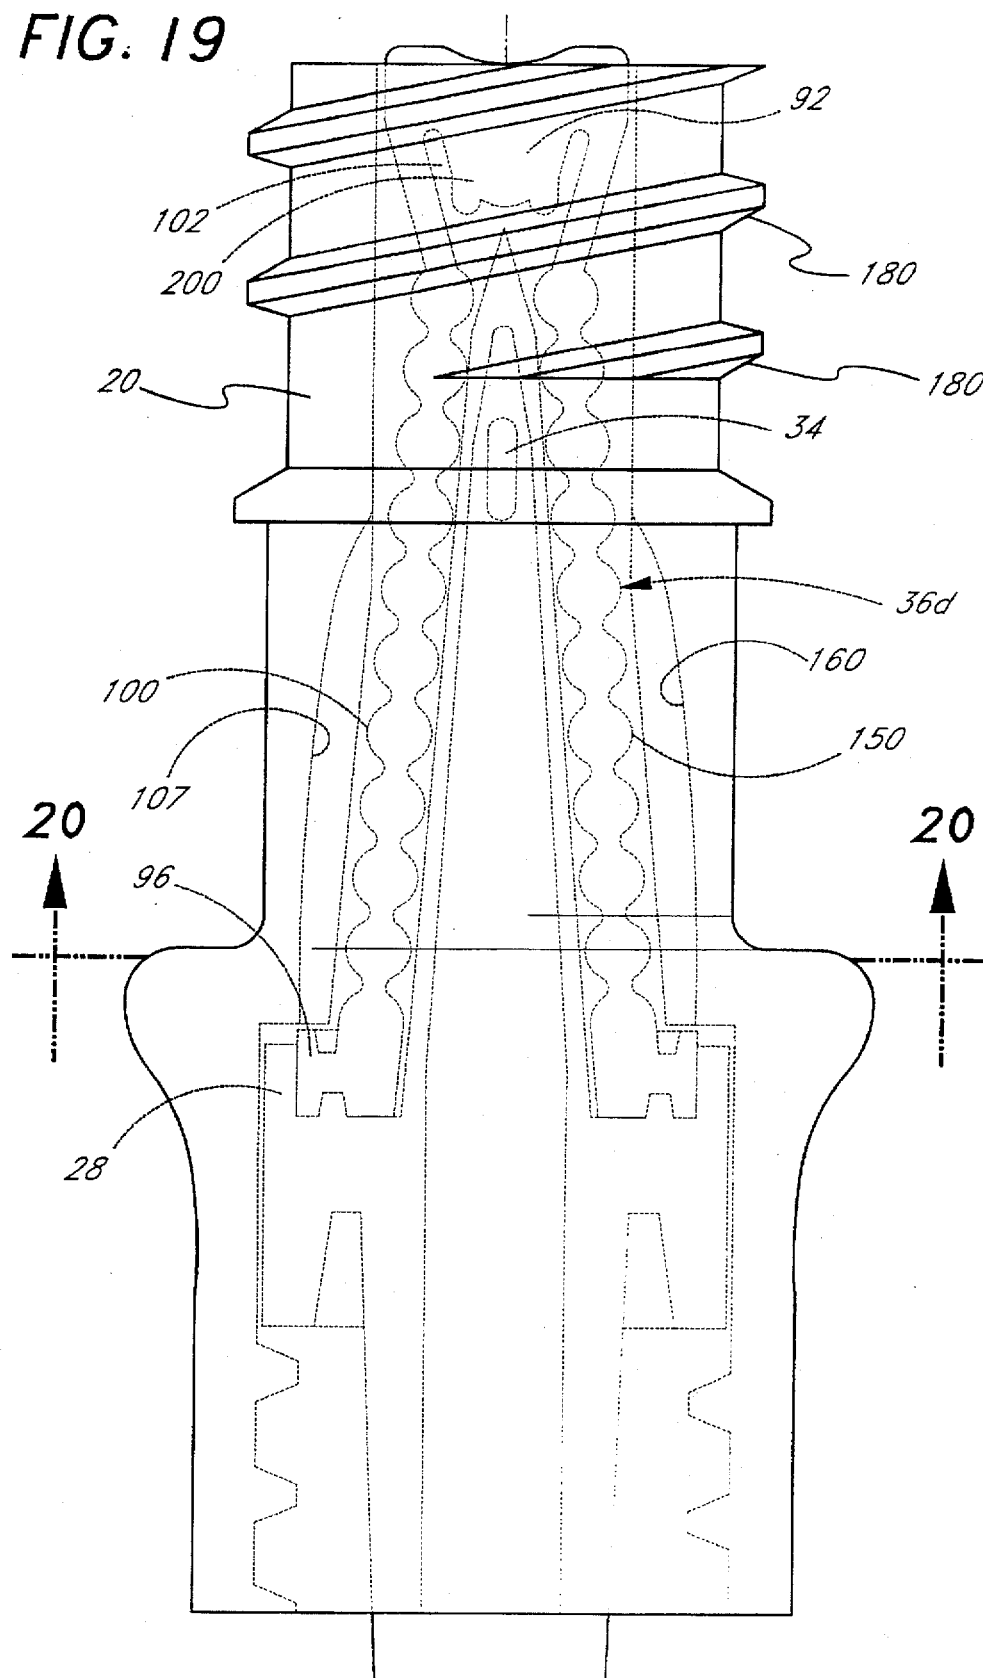


U.S. Patent

Nov. 11, 1997

Sheet 17 of 19

5,685,866

FIG. 20

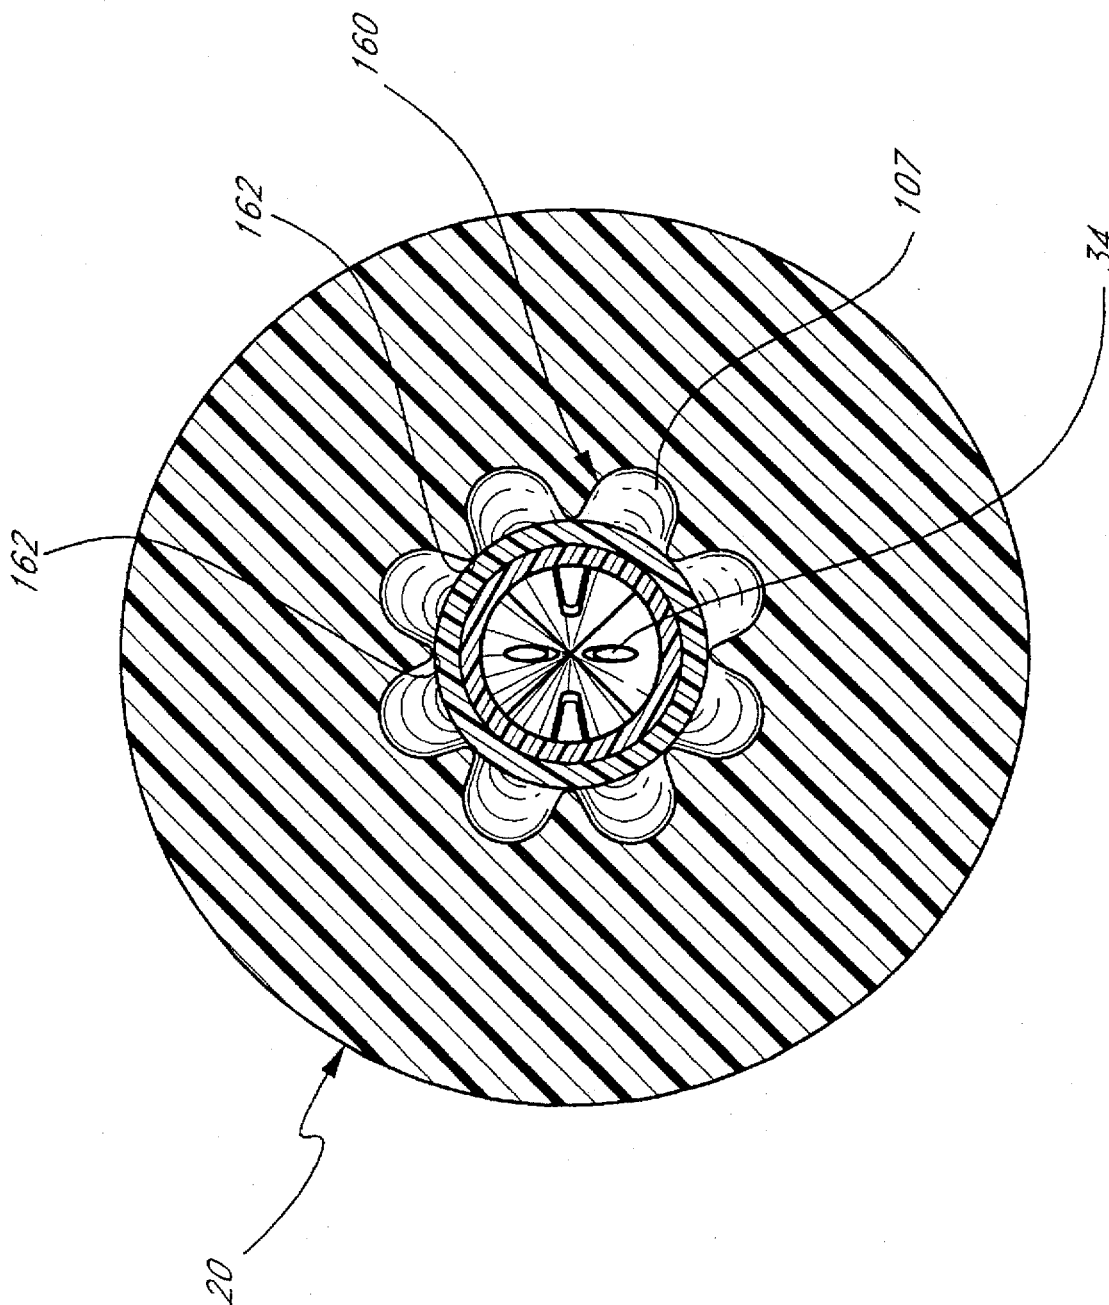

U.S. Patent

Nov. 11, 1997

Sheet 18 of 19

5,685,866

FIG. 21


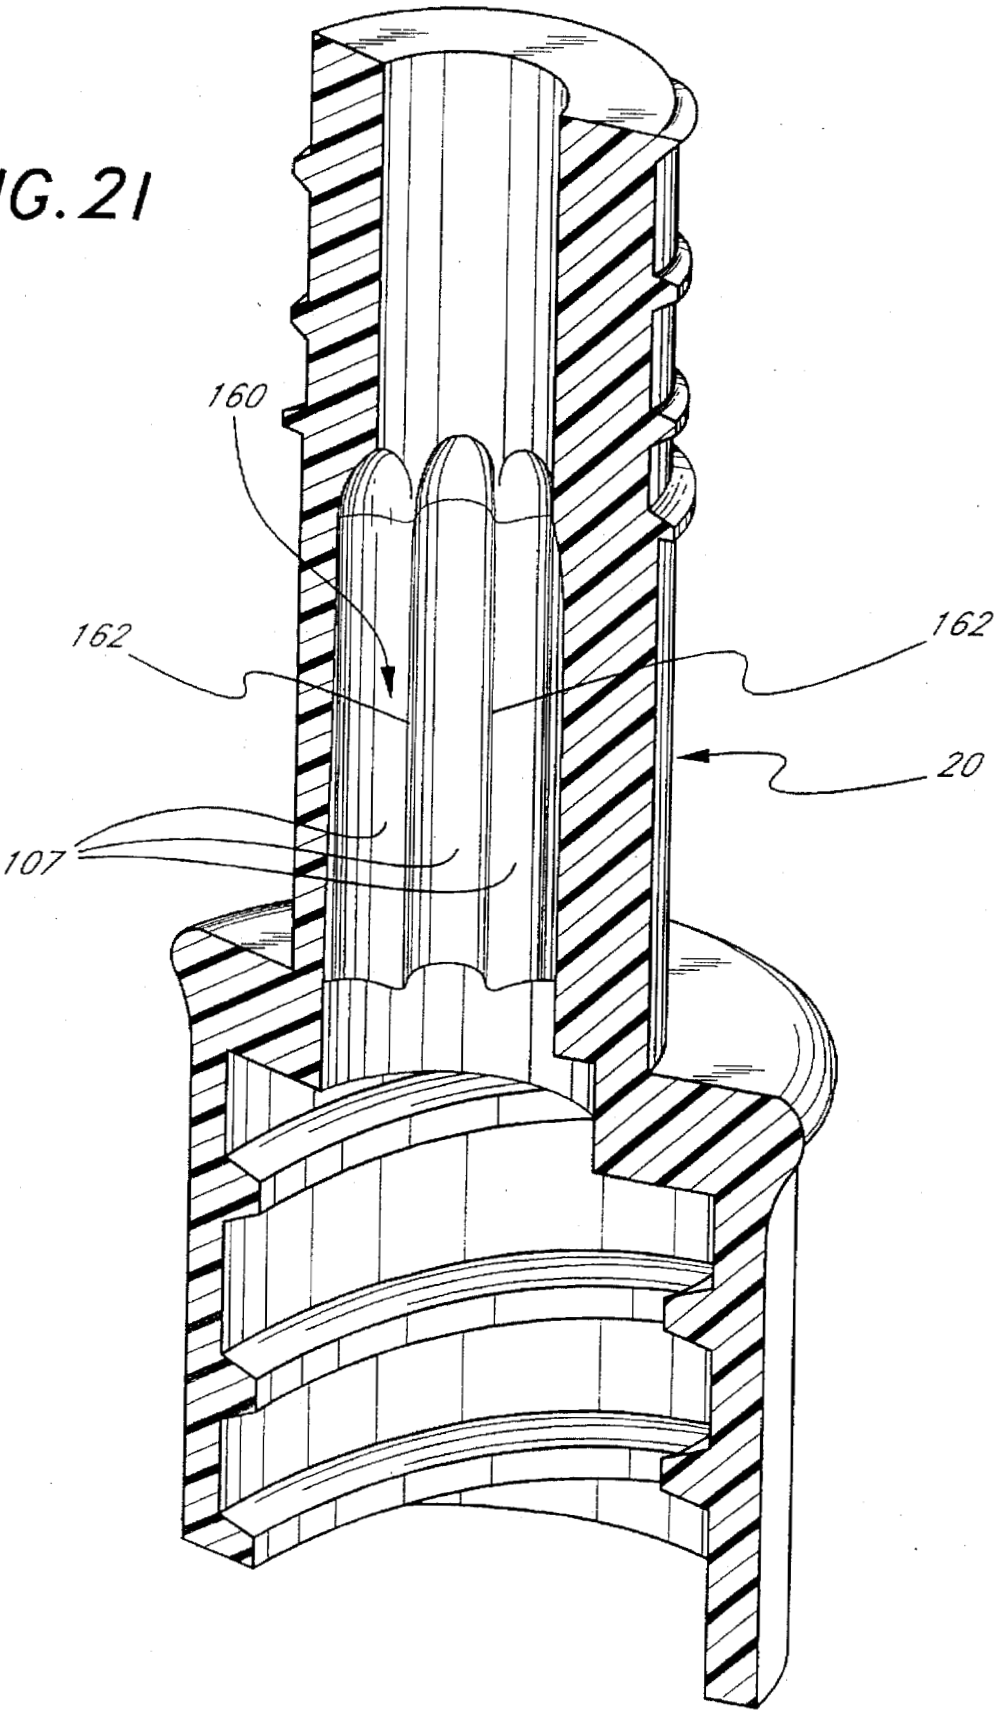


FIG. 22

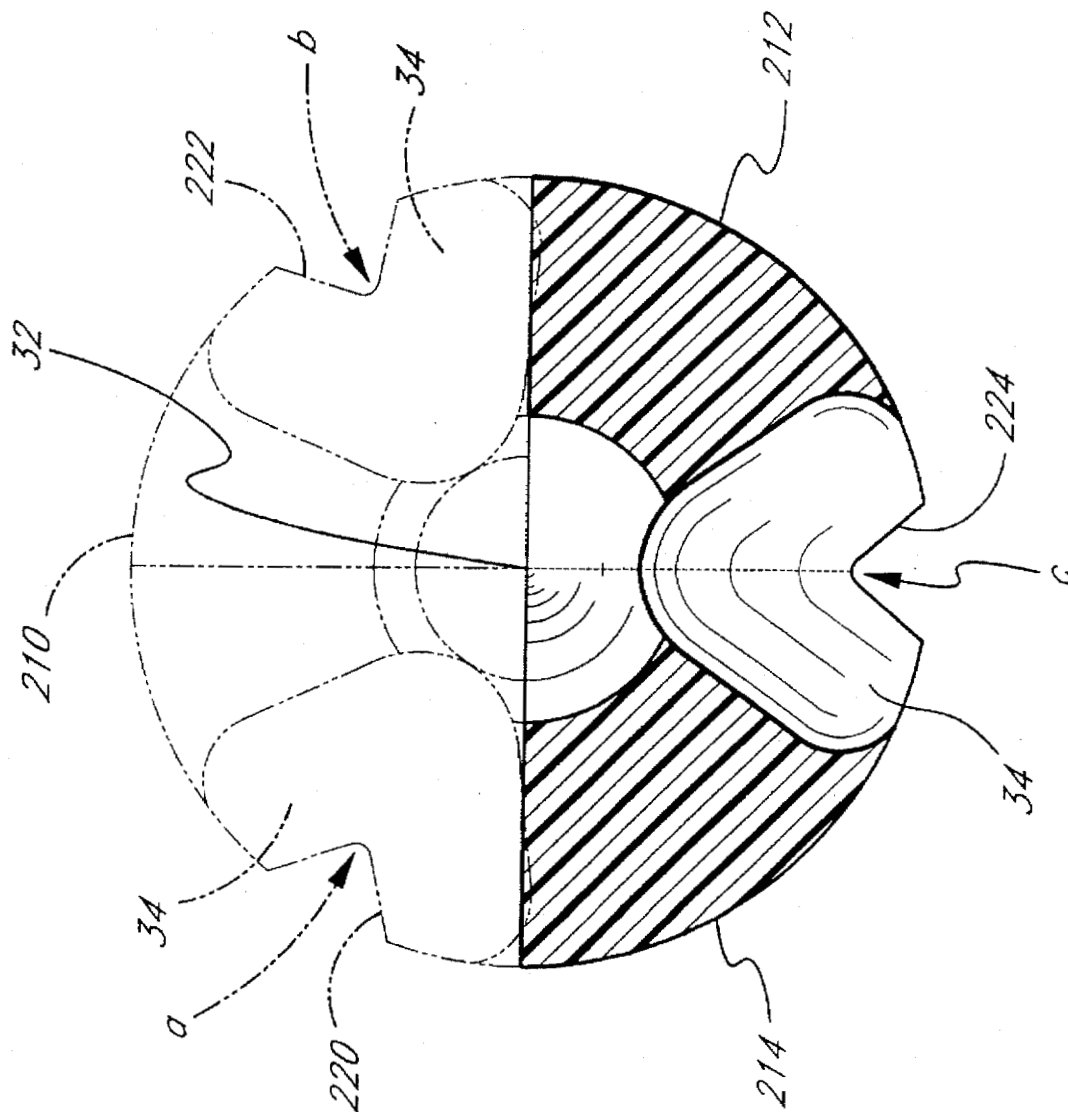

5,685,866

1

MEDICAL VALVE AND METHOD OF USE

This application is a continuation of U.S. application Ser. No. 08/096,659, filed Jul. 23, 1993, which is a continuation-in-part of International Application No. PCT/US92/10367, filed Dec. 1, 1992, now abandoned, which is a continuation-in-part of U.S. application Ser. No. 07/813,073, filed Dec. 18, 1991, now abandoned.

BACKGROUND OF THE INVENTION**1. Field of the Invention**

This invention relates to a closed, patient access system which automatically reseals after administering medication using a standard medical implement that directly connects with the system without the need of any intermediary needles, caps or adaptors. A two-way valve eliminating dead space is used which includes a seal which, upon being compressed by the medical implement, is pierced to open the valve and reseals upon being decompressed, maintaining a fluid tight seal even at high pressures and after repeated uses.

2. Background Discussion

The manipulation of fluids for parenteral administration in hospital and medical settings routinely involves the use of connectors and adaptors for facilitating the movement of fluids between two points. Most fluid connectors and adaptors employ needles to pierce a septum covering sterile tubing or to pierce the septum of a medicament container of fluid. Fluid then passes from the container or fluid filled tubing into a syringe or second set of tubing. These connectors and adaptors often have mechanical or moving parts. Since the ready passage of fluids through the connectors and adaptors is often critical to patient survival, it is imperative that the connectors and adaptors function reliably and repeatedly. Adaptors and connectors that malfunction during use may be life-threatening. The more mechanical or moving parts such as springs and diaphragms, the more likely that they will function improperly. Improper functioning can result in the introduction of air embolisms into a patient. Thus, the fewer the mechanical parts, the more these connectors can be relied on and the better they will be accepted by the medical community.

Many connectors or valves, especially those employing several mechanical components, have a relatively high volume of fluid space within them. This "dead space" within the device prevents accurate introduction of precise fluid volumes and provides an opportunity for contamination upon disconnection of the device. Connectors and adaptors often include valves that permit or interrupt the flow of fluid along the course of fluid travel. Several of those commonly in use employ metal needles to puncture sterile seals. Such connectors are generally designed to accommodate fluid flow in one direction. This means that the fluid line must have connectors and tube aligned in complementary directions. These connectors often require further manipulation if, for example, the valve is inadvertently assembled in a direction that will not facilitate fluid flow. These manipulations increase handling, thereby increasing both the risk of contamination and the amount of time required to establish the fluid connection.

Metal needles employed as part of connector devices increase the risk of puncture wounds to the user. The needles used in these devices often have through-holes placed at the tip of the needle. Connection of the valve with a flow line involves piercing the needle through a sealed septum. Through-holes placed at the needle tip can core the septum and release free particulates into the flow line. Such an event

2

can prove fatal to a patient. Such through-holes may also become clogged easily with material from the septum.

Reusable connectors and adaptors are preferred for medical applications since components must often be added or removed from a fluid line connected to a patient. Reusable connectors, however, are difficult to keep sterile. Sometimes caps are employed to cover the connector to keep it sterile. Frequently, these caps are lost, or simply not used because they are not readily available when needed.

A closed, patient access system that is easy to use and employs only a valve device in communication with the patient that need not be capped or interconnected with the medical implement through a needle or adaptor, is swabbable, is sufficiently durable to maintain its function after several manipulations, and maintains a fluid-tight seal at high pressures, would be of great benefit to the medical community.

SUMMARY OF THE INVENTION

The valve of this invention has several features, no single one of which is solely responsible for its desirable attributes. Without limiting the scope of this invention as expressed by the claims which follow, its more prominent features will now be discussed briefly. After considering this discussion, and particularly after reading the section entitled, "DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS," one will understand how the features of this invention provide its advantages, which include safety, reliable and repeatable performance, elimination of dead space, simplicity of manufacture and use, and employment of a valve that is swabbable after use to provide sterility and has a fluid-tight seal at high pressure.

This invention is a closed, patient access system which automatically reseals after administering medication using a medical implement that directly connects with the system without the need of any intermediate needles, caps or adaptors. A two-way valve is employed utilizing a reusable seal that may be repeatedly pierced by an enclosed, protected, non-metallic spike rather than an exposed metal needle. The valve facilitates fluid, particularly liquid, transfer while maintaining sterility. The valve is easy to use and is capable of locking in place. After use, the valve is swabbed in the conventional manner with a suitable substance to maintain sterility. The design of the valve avoids accidental needle sticks. As will be discussed in detail below, the valve is useful as a medical connector or adaptor to enable liquid flow from a sealed container.

The first feature of this invention is that the valve has a body including wall structure defining an internal cavity having a proximal end and a distal end. The cavity has an open space into which the seal is pushed, and preferably has a plurality of radial indentations in the wall structure that are adjacent the seal to accommodate the expansion of the seal upon compression. The proximal end has an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through the delivery end. In most applications, the delivery end of the implement is tapered, and the wall structure adjacent the opening is tapered inward so that the wall structure and the tapered delivery end fit snug against each other upon insertion of the delivery end into the opening. The proximal end of the cavity preferably is adapted to fit snug with an ANSI (American National Standards Institute, Washington, D. C.) standard end of the medical implement. Typically, the implement is a syringe, a connector or inlet/outlet of an IV set, or any one of a wide variety of conduits used in medical applications.

5,685,866

3

The second feature is that the spike has a tip with at least one hole located at or near the tip, and a passageway in communication with the hole that allows fluid to flow through this hole. The spike is seated inside the cavity such that the tip is inward of the proximal end and is enclosed within the cavity. Preferably, the hole is in a side of the spike adjacent the tip and is elongated, having a size of 18 gauge or greater. The tip may be sharp or slightly rounded. More than one hole is desirable for many applications, and three, symmetrically located holes inward of the proximal end are preferred. The spike may include at least one rib which allows air to enter a space between the seal and the spike, thereby facilitating the sealing of the opening when the implement is removed. The spike may have a substantially conical shape, and the seal has a complementarily, substantially conical shaped cavity within it conforming to the shape of the spike. The spike is disposed within this conical cavity and the seal covers the tip. The tip may be imbedded in the proximal end of the seal or withdrawn into the conical cavity. Preferably, the tip of the spike has a plurality of facets which meet within a recess. The preferred spike should be able to penetrate the seal repeatedly without tearing the seal. Rough edges at the tip may present a tear problem. During injection molding of the preferred plastic spike, facets of the tip will abut along a "parting line," and could form a rough edge which may tear the seal. This problem is avoided where the parting line is buried in a recess. Any rough edge at this parting line is disposed within a recess, so the seal material moves over the recess and does not contact the rough edge.

The third feature is that the resilient seal is adapted to be moved into a compressed state upon insertion of the tip of the medical implement into the opening and returns to a decompressed state upon removal of the tip. The seal in the decompressed state has a section which fills essentially completely a portion of the cavity adjacent the opening. The seal section bears against the wall structure near the opening to seal the opening. In the compressed state, the seal section is pushed by the delivery end of the medical implement away from the opening and into the cavity. A fluid tight seal is maintained between the seal section and the wall structure as the seal is moved into the compressed state. The seal section bears against the wall structure as the seal is moved inward into the cavity by the tip of the medical implement. And most importantly, the delivery end and the seal are adapted to engage so that when the tip of the spike pierces the seal there is essentially no dead space between said delivery end and the seal. Consequently, a predetermined dosage amount of medication is transferred in its entirety to the patient using this invention, with none to the prescribed amount being collected in dead space in the valve. The delivery of an exact amount of medication may be critical in some situations when chemotherapeutic agents are being administered or small children are being treated.

A fluid tight seal is maintained over repeated opening and closing of the valve, and the seal has on its external surface a recess which provides an air pocket to facilitate the movement of the seal. Preferably, the seal presents an essentially flush surface with the proximal end of the cavity. In one embodiment, the proximal end of the seal is substantially flat, the seal is made of a material having a hardness of from 30 to 70 Shore units such as, for example, a silicone polymer. The seal may include a cup-like flange adapted to engage the body near the proximal end of the cavity. A preferred embodiment of the seal comprises a series of O-ring elements stacked together and connected to form a unitary structure. The O-ring elements have increasing diameters, with the smallest diameter element being adja-

4

cent the proximal end of the cavity. The proximal end of the seal may be precut to form a tiny orifice therein that allows the tip of the spike to pass therethrough easily upon compression of the seal. Preferably, the proximal end of the seal has a truncated conical shaped segment disposed within the cavity. The seal may also have a centrally located, anti-vacuum, saucer like depression therein, which does not interfere with the ability of the exposed, proximal end of the seal being swabbed when desired.

The fourth feature is that the body and spike are two separate components of the valve that are securely attached to each other by assembly of, and interlocking, of the body and spike. The body has a first locking element near the distal end of the cavity, and the spike has a second locking element adapted to interlock with said first locking element upon assembly. The seal has a lip extending beyond the distal end and positioned between the first and second locking elements so that, upon assembly, the lip is compressed between the locking elements to provide an essentially fluid tight seal upon interlocking.

The fifth feature is that the medical valve includes a support member connected to the spike which seals off the distal end of the cavity. The support member may have a Luer-Lock type connector element that enables the valve to be removably attached to, for example, a fluid line connected to a patient. The support member may also be in the form of an adaptor that enables the valve to be removably attached to a fluid dispenser or container. When used to dispense fluids from a container, the spike has a pair of opposed tips, respectively at the distal and proximal ends of the spike. The tip at the distal end of the spike pierces a cover member which seals the container. A radial slit on the adaptor enables it to deform reversibly sufficiently to fit snugly onto said container.

The sixth feature is that the seal has a proximal end including a pressure responsive element disposed on an inner surface of the seal adjacent the opening. The pressure responsive element in the decompressed state closes any orifice in the seal at the proximal end of the seal to provide an essentially fluid-tight seal while in the decompressed state. The pressure responsive element enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve is connected to a patient's artery. The valve of this invention will remain closed even when the pressure inside the valve is above 6 pounds per square inch (psi), and it can withstand pressures above 30 psi. Typically, the pressure responsive element is a section of the seal having an entryway into a precut orifice. This section has a substantially cylindrical configuration and is surrounded by an annular space which is filled with pressurized fluid. The center of the member and the annular space are coaxial with the entryway to the orifice. The pressurized fluid fills the annular space to apply pressure that compresses the cylindrical section to tightly close the entryway to the orifice. Preferably, the pressure responsive element has an anti-tear element.

In accordance with this invention, a known, prescribed, predetermined amount or dosage of medication may be transferred from the remote source to the patient directly, so that essentially none of said predetermined amount is collected in dead space in the valve. In other words essentially all the prescribed dosage is received by the patient and not lost in the valve. Thus, this invention also includes a method of transferring fluid from a remote source to a patient. This invention also includes transfer of fluid from the patient to a remote source. This is possible because the valve of this

5,685,866

5

invention provides two-way communication. The fluid is transferred to the patient by applying pressure the fluid as it passes through the implement so that the pressure applied to the fluid is greater than the pressure of fluid in the patient, enabling transfer from the remote source to the patient. To achieve transfer of fluid from the patient to the remote source, the pressure of fluid in the patient is greater than the pressure at the remote source, causing fluid to flow from the patient to the remote source. This invention also includes a method of transferring fluid in a container having an open mouth covered by a cover member which seals the open mouth. The fluid is caused to flow from the container through the passageway by creating a differential in pressure. Preferably, the valve has an adaptor having a radial slit for allowing the adaptor to deform reversibly sufficiently to fit snugly onto said container.

BRIEF DESCRIPTION OF THE DRAWING

The preferred embodiments of this invention, illustrating all its features, will now be discussed in detail. These embodiments depict the novel and non-obvious method and valve of this invention shown in the accompanying drawing, which is for illustrative purposes only. This drawing includes the following Figures, with like numerals indicating like parts:

FIG. 1 is a perspective view of the first embodiment of the valve of this invention.

FIG. 2 is an exploded perspective view of the valve shown in FIG. 1 illustrating the spike, seal, and the body or housing components of the invention.

FIG. 3 is a longitudinal cross-sectional view of the assembled valve of FIG. 1.

FIG. 4 is a schematic, longitudinal, cross-sectional view of the assembled valve of FIG. 1 before compressing the seal.

FIG. 5 is a schematic, longitudinal, cross-sectional view similar to FIG. 4 showing the valve during compression of the seal.

FIG. 6 is a perspective view of a second embodiment of the invention.

FIG. 7 is a longitudinal cross-sectional view of the valve of FIG. 6.

FIG. 8 is a schematic illustration of an ANSI delivery end of a medical implement compressing the seal of the valve of this invention.

FIG. 9 is a side elevation view, partially in cross-section, of a third embodiment of the seal.

FIG. 10 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using the seal of FIG. 9.

FIG. 11 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fourth embodiment of the seal.

FIG. 12 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fifth embodiment of the seal.

FIG. 13 is a longitudinal cross-sectional view of a sixth embodiment of the seal.

FIG. 14 is a longitudinal section of the seal shown in FIG. 13 used in connection with the spike device shown in FIG. 2.

FIG. 15 is a longitudinal partial cross-sectional view of a seventh embodiment of the seal of this invention.

FIG. 16 is a longitudinal cross-sectional view, after assembly, of the embodiment of the valve shown utilizing the seal of FIG. 15.

6

FIG. 17 is a longitudinal cross-sectional view, after assembly, of the eighth embodiment of the valve of this invention.

FIG. 18 is a longitudinal cross-sectional view, after assembly, of the ninth embodiment of the valve of this invention.

FIG. 19 is a side elevation view, after assembly, of the seal and spike shown in FIG. 14 connected to the body or housing shown in FIGS. 20 and 21.

FIG. 20 is a cross-sectional view taken along line 20—20 of FIG. 19.

FIG. 21 is a perspective view, with sections broken away to show the wall structure of the cavity containing the seal shown in FIGS. 13 and 14.

FIG. 22 is a greatly enlarged, cross-sectional view taken along line 22—22 of FIG. 14.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

The term "proximal" is used to denote the end of the valve and other components at or near the spike tip 32 in FIGS. 2 through 5, 10 through 12, 14, and 16, and at or near the spike tip 60 in FIG. 6, and at or near the seal cap 92 in FIGS. 8, 9, 13 through 19. The term "distal" is used to denote the opposite end of the valve, or spike tip, or seal. The term "medical implement" is used to denote any medical tool known to those of skill in the art that can connect to the present invention and facilitate the passage of fluids, particularly liquids, through the instant invention. Examples of medical implements that are contemplated include, but are not limited to, tubing, conduit, syringes, IV sets (both peripheral and central lines), piggyback lines, and other components which can be used in connection with a medical valve. Medical implements are commercially available in standard sizes. Thus, either or both ends of the valve of this invention can be provided with fittings to accommodate such standard size medical implements.

As best shown in FIGS. 1 and 2, the first embodiment of the invention, valve 10, includes a valve body or housing 12, a spike element 24, and a seal 36. The seal 36 is prepared from a resilient material that is flexible, inert, impermeable to fluid, and readily pierceable by the spike 26. In the embodiment shown in FIG. 13 depicting an alternate shaped seal 36d, this seal 36d has a precut slit 11 in its proximal end. This provides a tiny orifice through which the tip 32 of the spike element 24 may easily pass, yet still provides a fluid tight seal upon withdrawal of the spike element. These three components are assembled, as depicted in FIG. 3, with the spike element 24 enclosed to prevent accidental sticks. FIG. 2 illustrates how the housing 12, seal 36, and spike element 24 are attached without the need to use any adhesive or other bonding agent or process. Mechanical connection which provides a fluid tight closure is attained as is discussed subsequently. As shown in FIGS. 4 and 5, the seal 36 moves within the housing 12, being pierced by the spike element 24 to expose the tip 32 of the spike element 24 to allow fluid to flow through the valve 10.

Referring to FIG. 1, one preferred embodiment of housing 12 has a bell-shaped skirt 16 and an upper, preferably cylindrical, conduit 20. The skirt 16 is integral with, and connected by an annular ring 14, to the upper conduit 20. The skirt 16 creates a shield for an inner conduit 18 of the spike element 24. This inner conduit 18 is preferably cylindrical in shape, and slightly tapered. Inner conduit 18 and upper conduit 20 comprise aligned hollow tubes so that inner conduit 18 and upper conduit 20 are in fluid commu-

5,685,866

7

nication with one another when the spike element 24 pierces the seal 36. There is an annular lip 25 surrounding a circular opening 25a in the top of the conduit 20 (see FIG. 2).

In the first embodiment, the upper conduit 20 is adapted to receive the tip or nose 48 of an ANSI standard syringe 46 (see FIGS. 4 and 5). It is, however, contemplated that the outer diameter of the upper conduit 20 can be of any size to accommodate the attachment of other connector devices thereto. Advantageously, the proximal end of the upper conduit 20 can be equipped with a locking mechanism to facilitate locking of the valve 10 to a variety of connector devices. For example, referring to FIG. 1, locking ears 22 near the proximal lip 25 of housing 12 are preferably provided such that the housing 12 can be locked into any compatible Luer-Lock device known to those with skill in the art. For example, referring to FIG. 19, conventional Luer-Lock threads 180 can be provided on the outer diameter of upper conduit 20.

Referring to FIG. 2, the spike element 24 has at its distal end the inner conduit 18 and at its proximal end a hollow spike 26 which is integral with the inner conduit. The inner conduit 18 and spike 26 present a continuous passageway for fluid during use. An annular cuff 28 on an intermediate portion of the spike element 24 is integral with, and interconnects, the inner conduit 18 and the spike 26. As illustrated in FIG. 3, the rim 28a of the cuff 28 abuts the underside of the inner ring 14, and has an annular detent 28b that snaps into an annular groove 14b in the underside of the ring. The cuff 28 serves two functions. First, it serves as an attachment device to the underside of the annular ring 14. Second, it serves as a support and attachment device for the seal 36.

The hollow spike 26 has a tapered conical shape, ending in a sharp, pointed tip 32. Preferably, along the length of the spike are raised, protruding ridges 30. These raised ridges 30 extend from the surface of the spike preferably between 0.2–2.0 mm. The ridges 30 are preferably aligned along the length of the spike as illustrated in FIG. 2. These ridges 30 serve to break any vacuum created when the spike 26 is sealed as described hereinbelow. Modifications to the alignment and orientation of the ridges are discussed hereinbelow in association with their function. Just distal the spike tip 32, there is situated at least one longitudinal through-hole 34 to permit fluid communication between the inner conduit 18 and the upper conduit 20. Preferably, there are three through-holes 34 within about 0.200 inch from the spike tip 32. These through-holes 34 may be of any size, however, the larger the size of the through-holes the greater the fluid flow rate through the valve 10. In a preferred embodiment, the size of the through-holes 34 are 18-gauge to provide a flow rate three times that of a standard 18 gauge needle.

The seal 36 has a seal cap 40 with a generally flat top surface 40b, an outwardly tapered sidewall 38, and a lower lip 42. Its interior is hollow to provide the conically shaped cavity 37 (FIG. 3). Thus, the seal 36 slips easily over the spike element 24 to fit snugly within the cavity 37. The seal lip 42 is seated within the annular cuff 28 and wedged between the cuff and the underside of the ring 14. There are longitudinal grooves 43 (FIG. 2) along the length of the seal 36 which provide air pockets that facilitate compression of the seal 36 during use. The grooves 43 may be of variable shape or size to facilitate seal compression. In the first embodiment, there is a single groove 43 which completely surrounds the seal 36 between the seal cap 40 and the lip 42.

The base of the seal 36 has a width such that the seal lip 42 fits snugly into the annular cuff 28. The hollow interior

8

or cavity 37 (FIG. 3) of the seal 36 is preferably tapered to conform internally to the shape of the spike 24, having a wall portion 44 which contacts the spike 24 distal seal cap 40. The exterior of the seal 36 is sized and shaped to fit inside the upper conduit 20 of the housing 12. The cap 40 reseals the valve 10 when the top surface 40b is above the through-holes 34. Preferably, the cap 40 substantially fills the opening 25a in the top of the conduit 20. Thus, after assembly, the top surface 40b of the seal cap 40 is essentially flush with the lip 25, so that the lip 25 and seal cap 40 can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve 10. It is important that the surface 40b be exposed so that it may be swabbed with a disinfectant.

As best shown in FIG. 3, the spike 24, with contiguous inner conduit 18, is affixed to the housing 12 through the association of the external portion of annular cuff 28 and the internal portion of annular ring 14. Although not necessarily required, these two pieces may be affixed by any one of a variety of methods known to those of skill in the art including, but not limited to, heat sealing, glue, pressure lock, bonding or the like. The seal 36 fits into the annular cuff 28 and is held in place by an internal lip 27 along the internal portion of the annular ring 14 of the housing 12. The length of the spike 24 is such that, after assembly, the tip of the spike rests below the plane defined by the lip 25 of the housing 12. Preferably, the spike tip 32 is approximately from 0.525" to 0.1" below the lip 25 of the housing 12. The seal 36 fits snugly against the spike 24 and is essentially flush with the lip 25 of the housing 12. The spike tip 32 is thus embedded within the seal cap 40 prior to use or may be approximately 0.025" distal the seal cap 40 when the valve 10 is in the closed position. The inner conduit 18 is partially shielded by the bell shaped skirt 16 of the housing 12 (see FIGS. 1–3). The inner surface of the bell shaped skirt 16 preferably has protruding threads 44 as an optional locking mechanism for attaching a medical implement thereto. Further, other medical devices can be pressure fit over the outer portion of inner conduit 18 without direct association with the protruding threads 44.

During use, the invention is designed to be adapted as a two-way valve. The orientation of the valve is independent to fluid flow and dependent on the preferred orientation of the preexisting connections. Thus, the invention can be used as a valve connector for an intravenous central or peripheral piggyback connector in either orientation. Parenteral fluid is delivered to patients through tubing such that the liquid flows from a container through a needle into the patient. The containers are frequently changed or additional fluid bottles are added. The invention disclosed herein is designed to interconnect medical implements along the route of fluid delivery to the patient. However, the invention is also useful in any environment in which a resealable fluid valve is desired. During use, a connector of the appropriate size is fitted over the inner conduit 18. Locking can be achieved by a Luer-Lock mechanism, a pressure fit or any other locking mechanisms known to those with skill in the art, as described above. Thus, in one example, fluid passes from the inner conduit 18 into the spike 26. However, fluid flow is locked in place by the seal 36.

FIGS. 4 and 5 illustrate valve activation. In FIG. 4, the medical implement connecting to the proximal end of the valve 10 is a syringe 46. However, this connecting implement could be any number of medical implements known to those of skill in the art. The nose 48 of the syringe 46 is placed on the seal cap 40 inside the lip 25 of the housing 12. The application of pressure on the syringe 46 in the direction of the arrows, as illustrated in FIG. 4 creates pressure on seal

5,685,866

9

cap 40. The resulting downward pressure compresses the seal 36. This pushes the tip 32 of the spike 26 through the seal cap 40 to expose the through-holes 34. Compression is facilitated by the grooves 38. Fluid is now able to flow into the syringe 46, or vice versa, depending on whether fluid is to be withdrawn from the patient or medication injected into the patient. FIG. 5 shows valve 10 opened by insertion of the nose 48 of the syringe 46 into the opening 25a. A syringe plunger 49 in the syringe 46 is retracted thereby creating a vacuum to draw fluid through the valve 10 into the syringe. For intravenous applications, the valve 10 can be orientated in the position diagrammed in FIGS. 4 and 5, or it can be rotated 180° such that fluid flows in the opposite direction.

Upon removal of the syringe from spike 26, as shown in FIG. 4, the seal 36 is free to return to its original shape and cover through-holes 34. The ability of the seal 36 to return to its original shape is determined by the resiliency of the material used to prepare the seal 36. In addition, the ability of the seal 36 to return to its original shape is facilitated by the protruding ridges 30 formed on the external surface of the spike. During compression, a vacuum may form in the area between the spike 26 and the seal 36, thereby preventing the seal 36 from returning to its original position. The protruding ridges permit air to pass along the spike/seal interface to prevent vacuum formation and allow free return of the seal. The ability of the seal 36 to deform reversibly and return to its original position is particularly useful because (1) it immediately stops fluid flow through the valve 10, (2) it covers the recessed spike 26 to maintain its sterility, and (3) it reduces the risk that the spike could inadvertently pierce another object or person. In addition, since the valve 10 lacks movable parts, except for the seal, it is unlikely that when the seal 36 is pushed down, the valve 10 would fail to function.

Advantageously, the through-holes 34 are located relatively low on the spike 26. Thus, the through-holes 34 are sealed relatively early in the process as the seal 36 returns to its original configuration with the valve 10 is closed. In one preferred embodiment the through-holes 34 are located 0.075" below the spike tip 32 (see FIG. 2). Additionally, the through-holes 34 are sealed even if the seal 36 does not fully return to its original configuration depicted in FIG. 4. Further, the ability of the seal 36 to return reversibly to its original position permits the reuse of the connector valve 10. Following disconnection, and before reuse, the surface of pierced seal cap 40 is essentially flush with the housing 12. Thus, this flush surface can, advantageously be sterilized with alcohol or other surface decontaminating substances. The skirt 16 and upper conduit 20 advantageously shield both connections from the surrounding environment to protect the sterility of the connection. Further, both the skirt 16 and upper conduit 20 function as collection reservoirs to prevent fluid from dripping from the valve 10 during manipulation.

A cover cap (not shown) can be supplied to fit over the upper conduit 20 as further protection for the seal surface between use. Such a cover cap, however, is not needed to maintain sterility since the seal 36 may be swabbed with a disinfectant after each use. The reversibility of the seal 36 makes the valve 10 particularly attractive as a connector valve to provide fluid communication between two fluid lines. Therefore, the present invention provides for placing a first fluid line in communication with a second fluid line using the valve disclosed herein. The reversibility of the valve 10 permits multiple fluid lines to be successively added, for example, to a fluid line in direct communication with a patient's vein. Since the valve is easily sterilizable

10

and sealable, fluid lines can be added and removed without disconnecting venous contact.

The valve 10 is preferably prepared from a hard plastic, but it is additionally contemplated that the valve could be prepared from other medically inert materials known to those in the art. The spike element 24 is preferably prepared from the same material as the housing 12. One particular advantage of this invention is that it does not rely on the use of metal needles. This dramatically reduces the risk of skin puncture during use and manufacture. Further, the upper conduit 20 serves as a shield to the spike 26 such that skin puncture is further reduced. The spike 26 need only be strong enough to penetrate the seal cap 40, or if necessary, to pierce a connecting septum.

In the embodiment of the invention illustrated in FIGS. 2-4, the through-holes 34 are placed distal spike tip 32. This placement provides two important advantages. First, the placement of the through-holes 34 facilitates resealing of the valve 10 after use. Second, if the through-holes were placed at the spike tip 32, the holes 34 may core the seal cap 40 thereby introducing seal particulate into the fluid flow and possibly plugging the holes 34. Thus, the longitudinal placement of the through-holes distal spike tip 32 prevents the introduction of particulates into the fluid path and/or plugging of the through-holes 34. It is additionally contemplated that the number and diameter of the through-holes 34 can be adjusted to accommodate different fluid velocities. In a preferred embodiment, the preferred velocity of fluid passing through the through-holes 34 is equal to or greater than the flow rate through an 18 gauge needle. Through-holes larger than 18 gauge will, of course, facilitate greater fluid velocities.

An important advantage of the invention is that the valve 10 has very little dead space, thus the volume of liquid entering into the valve is substantially equivalent to the volume of fluid leaving the valve. Further, the total equivalent fluid volume of the valve is very small such that the volume of fluid flowing through the system in order to place the valve in fluid communication with a medical implement such as a syringe 46 is substantially zero.

ALTERNATE EMBODIMENTS

In another preferred embodiment of the invention, illustrated by FIGS. 6 and 7, a disposable sterile adaptor valve 50 is provided to function as a resealable lid for a container (not shown) of fluid. The fluid can thus be removed from the fluid container or permitted to flow from the container into a medical implement adapted to house fluid in a sterile manner. As is the conventional practice, an open mouth of the container will ordinarily be sealed with a cover member (not shown).

FIG. 6 shows an adaptor valve 50 having a body including an adaptor skirt 52. The adaptor skirt 52 will preferably fit snugly over the open mouth of the container. The skirt 52 may be of any size to accommodate a range of container sizes. A lengthwise slit 54 is preferably provided in at least one location along the length of the skirt to ensure a snug fit between the skirt 52 and the container. A chamber 56, preferably tubular in configuration, extends upward from the skirt 52 and is similar in construction and design to the upper chamber 20 of the first preferred embodiment. Similar to the first embodiment, the proximal portion of the valve contains a locking mechanism 59 that preferably comprises a Luer-Lock device or other locking device known to those of skill in the art.

As depicted in FIG. 7 a spike 58 extends upward through a tubular chamber 56. A spike tip 60 is preferably recessed

5,685,866

11

from a proximal lip 62 of the tubular chamber 56. In a closed position, this tip 60 is covered by a seal 64, which is essentially the same as seal 36. Protruding ridges 66 and seal grooves 68 facilitate seal compression in the open position and promote closure following use. Thus, in the closed position as illustrated in FIG. 7, the seal 64 covers the through-holes 70 to prevent fluid out-flow from the container. The adaptor valve 50 contains a second spike 72 which points in the opposite direction as spike 58. These spikes 52 and 72 are in fluid communication with each other. The spike 72 extends downward inside the adapter skirt 52. The two spikes preferably form one component of the valve 50 while the skirt 52 and upper chamber form a second component. These two components can be assembled in a manner like that of the valve 10. The spike 72, like the spike 58, has longitudinal through-holes 74 and a tip 76. The through-holes 74 are located inward of the tip 76. The adaptor valve 50 is thus useable with containers holding sterile medicament having a cover or septum seal at the open mouth of the container. Examples of containers with such seals contemplated for use with this invention include dosage bottles for intramuscular injector antibiotic containers or the like. However, it is also contemplated that the valve 50 can be adapted with its own seal and locking mechanism to permit the valve to be employed on a variety of containers for medicaments or other fluids. Medicaments in these types of containers are preferably maintained under sterile conditions and the volume and nature of the medicament is such that multiple aliquots are intermittently removed over time. If the medicament is reconstituted, then, during use, any covering over the opening on the container is removed to reveal the rubber septum. The adaptor valve 50 is placed over the septum and direct pressure is applied to pierce distal spike 72 through the septum and into the container. A syringe or the like can then be applied, as depicted in FIG. 4, in association with the first preferred embodiment, to withdraw fluid from the container. The pressure of the nose 48 over the spike 58 pushes spike tip 60 through seal 64. At the same time, seal 64 is pushed back and compresses. Compression is accommodated by seal grooves 68. Fluid is withdrawn from the container and the syringe is removed from the spike 58. Release of the pressure applied to seal 64 permits the seal to return to its original configuration. The spike ridges 66 facilitate seal reversibility.

Often the ingredients housed in containers are those that can be lyophilized at purchase. Lyophilized ingredients require reconstitution before use. If the medicament requires reconstitution before use, then sterile water, saline, or other fluid can be introduced into the container before fluid is extracted. The two-way nature of the valve permits this without any special adaptation. After the syringe is removed, the adaptor valve 50 automatically seals. Subsequently, aliquots can be removed from the container by syringe or the like. Alcohol or other compatible surface sterilizing agent can be used to wipe the lip 62 and seal 64 before each use. Similar to the first embodiment, it is additionally contemplated that a cap can be provided to fit over upper chamber lip 62 between use.

The adaptor valve 50 can be adapted to function as a medicament adaptor for an intravenous container. In this case, the adaptor valve 50 is placed on a medicament container for intravenous delivery and attached via tubing to an intravenous feed. Thus, the adaptor valve 50 can be placed in fluid communication with a connector valve of FIG. 1 to facilitate the flow of medicament from intravenous drip bottles.

An alternative embodiment of the seal, a seal 36a, is shown in FIG. 9. Seal 36a comprises a seal cap 92 at the

12

proximal end thereof and a seal lip 96 at the distal end thereof. A cup-like annular flange 95 is provided proximal seal cap 92. The seal cap 92 and seal lip 96 are connected by a seal wall consisting of a plurality of ringed wall portions 94 that expand and collapse in an accordion like fashion. During compression of the seal 36a, the diameter of the ringed wall portions 94 expand outward in the radial direction. There are air pockets 13a (FIG. 10) between ring portions 94 and the housing and air pockets 13b between spike 24 and seal 36a. The seal 36a contains a cavity 98 distal seal cap 92 and adjacent the ringed wall portions 94. The seal 36a interacts with spike 26 (FIG. 2) and other components of the present invention in a similar fashion to seal 36 of FIG. 2.

Referring to FIG. 10, the cup-like annular flange 95 may be stretched around the upper conduit 20 and held in place by an annular ring 97. This creates a trampoline like effect that assists returning the seal 36a to a decompressed state after withdrawal of a syringe (not shown). This embodiment has two advantages. First, the proximal end of the valve 10 can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve 10. Second, by affixing cup-like annular flange 95 to upper conduit 20 at the proximal end thereof with annular ring 97, the repeated deformation and reformation of the seal 36a is assisted.

An alternative embodiment of the seal, a seal 36b is shown in connection with the valve 10 in FIG. 11. The seal 36b is similar to the seal 36a and is comprised of seal cap 92, a side wall consisting of ringed wall portions 94 and a seal lip 96. It also has an outwardly extending ring 99 which is at a right angle with respect to the longitudinal axis of the valve 10. This ring 99 is used to attach the seal 36b to upper conduit 20. Preferably, an upper conduit annular plug 20' is inserted within upper conduit 20 to create a tight fit between perpendicular ring 99, a ledge 101 in the upper conduit 20, and the plug 20'. The ring 99 assists in the reformation of seal 36b to enclose spike 26 upon withdrawal of a syringe (not shown).

As shown in FIG. 12, the cup-like annular flange 95 and ring 99 may both be used in connection with the valve 10, to provide the seal 36c. This seal 36c, provides rapid reformation upon withdrawal of a syringe (not shown) and realizes the advantages of both the seals 36a and 36b.

Another alternative embodiment of the seal, a seal 36d, is shown in FIG. 13. In this embodiment, the seal 36d is comprised of seal cap 92, seal lip 96, and a side wall 150 comprised of circular tires 100 stacked in series one on top of an adjacent larger diameter lower tire. The circular tires 100 are preferably solid throughout the diameter of the cross-section thereof. These circular tires 100 will deform and reform upon, respectively, compression and decompression of the seal 36d, thereby exposing or covering a spike (not shown) as the case may be.

As mentioned above, preferably seal 36d has a precut slit 11 in the cap 92 lying along the longitudinal axis of the valve 10. The seal cap 92 has a unique configuration that insures that the slit 11 closes and is sealed upon withdrawal of a syringe (not shown) and reformation of the seal 36d. It includes an enlarged, internal, pressure responsive member 200 which is integral with the cap 92. Between the proximal end of the side wall 150 and the member 200 is an annular space 102 which is filled with the fluid in the cavity 98. This fluid is under pressure, for example at the blood pressure of the patient to which the valve 10 is attached. Referring to FIG. 14, fluid, for example the patient's blood, flows through the holes 34 in the spike 26, filling the cavity 102.

5,685,866

13

This fluid presses against the exterior of the member 200, closing the slit 11 when the seal is decompressed as shown in FIGS. 14 and 19. The pressure from this fluid creates a high pressure seal which prevents fluid from escaping valve 10 through the slit 11. There is a semi-cylindrical annular flange tear ring 104 on the end of the member 200 which advantageously extends the useful life of seal 36d.

Preferably, there is a tear ring 104 integral with the member 200 along the perimeter of the internal surface the member 200, and a slight saucer-like depression 204 in the external surface of the seal. The pressure responsive element in the decompressed state closes any orifice in the seal 36d to provide an essentially fluid-tight seal while in the decompressed state. The pressure responsive member 200 enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve 10 is connected to a patient's artery. The center of the member 200 and the annular space 102 are coaxial with the entryway 11a to the orifice 11. The pressurized fluid fills the annular space 102 to apply pressure that compresses the member 200 to tightly close the entryway to the orifice. In a preferred embodiment the distance from the entryway 11a to the proximal end of seal cap 92 is from 0.500 to 0.075 inches and more preferably approximately 0.100 inch.

As best illustrated in FIG. 22, the tip 32 is designed to avoid tearing the seal. Tip 32 has three facets 210, 212, and 214 which are joined with each other along parting lines a, b, and c. This junction of the facets 210, 212, and 214 frequently is ragged and will tear the seal 36d. This is prevented by the parting lines a, b, and c, or junctions, being disposed within recesses 220, 222, and 224, respectively, to provide "buried parting lines."

Another alternative embodiment of the present invention using the seal 36d is shown in FIG. 8 and FIGS. 19 through 21. In this embodiment, the inner wall 160 of the upper end of the conduit 20 is provided with at least one, and preferably, a plurality of radial indentations 107. The indentations 107 are elongated disposed generally parallel to the longitudinal axis of the valve 10 in a symmetrical, star-like configuration. Each indentation has opposed lateral edges 162 which engage the seal 36d upon compression of the seal 36d. The indentations provide space into which the seal 36d expands upon compression.

As best shown in FIG. 8, the wall 181 of the proximal end of the conduit 20 is tapered inward at the same angle as the nose 48 of the syringe 46. In accordance with ANSI standards, the taper is 0.006 inch per linear inch. The wall 182 of the syringe nose 48 bears against the wall 181 as the nose slides into the opening 25a to push the seal 36d inward compressing it and forcing the tip 32 of the spike 36 to enter the slit 11. The seal 36d expands upon compression to fill essentially completely the upper portions of the indentations 107. Some sections of the seal 36d are wedged between the edges 162 and other sections fill the indentations 107. As the liquid flows through the nose 48 through holes 34, air in the nose 48 is forced out of the nose 48 and expelled from valve 10 between walls 181 and 182. Thus, essentially the entire prescribed dosage is delivered through valve 10 to the patient. Fluid flows through the through-holes 34, but does not leak between either the seal 36d and the wall 181 or between the abutting walls 181 and 182.

FIGS. 15, 16, 17, and 18 depict embodiments of seals, namely, seal 36e, seal 36f, and seal 36g, which are substantially the same as the seals 36a (FIG. 10), seal 36b (FIG. 11), and seal 36c (FIG. 12), except the side wall 150 employing the circular tires 100 is used in place of the accordion wall portion 94.

14

Other components of the present invention interact with the various embodiments of the seal in a similar fashion to their interaction with seal 36 of FIG. 2. Prior to use of valve 10, it is preferable that the seal caps 40 or 92 be pierced centrally by a steel needle in the axial direction, precutting the seal to provide the slit 11 in order to allow for more rapid decompression and reformation of the seal upon piercing by the spike 26. The seals are advantageously formed from a material which can repeatedly reseal and prevent fluid from flowing around the seal material. The seal 36 should also be capable of being forced down and then spring back into position to reseal the valve. Material that is too soft will reseal effectively; however, will not be capable of springing back after opening of the valve. Material that is too hard will provide sufficient spring force; however, will not effectively seal. Thus, in a preferred embodiment, the seal is formed from a silicone having a hardness in the range from 30-70 Shore durometer units, and more preferably in the range 40-50 Shore durometer units. A cure silicone polymer in the preferred hardness range is available from Wacker Silicone Corp. of Adrian, Mich. In some embodiments of the invention, it is desirable to provide additional lubricity to the seal 36 to allow it to spring back and reseal more effectively. Dow Chemical Co. produces a silicone formulation with silicone oil built in to provide this additional lubricity.

In general, the closing of the valve 10 is provided not by the side wall of the seal 36 which immediately covers the through-holes 34, but by the seal cap 40, or seal cap 92 filling the proximal end of the cavity 98 and the opening 25a. Thus, the seal caps 40 and 92 are sufficiently thick to reseal the opening 25a effectively after valve closure. However, the seal caps 40 and 92 should also be sufficiently thin to allow them to readily return to the closed position. Preferably the thickness of the caps 40 and 92 ranges between 0.075 and 0.500 inch and more preferably may be approximately 0.100 inch.

The valve disclosed in this invention can be provided in a sterile and disposable form such that after its use in a given installation is exhausted, the device is discarded. However, as described above, in any given installation, the device can be reused multiple times. Since the device does not employ needles, there is little chance that the device will inadvertently cause skin puncture. Therefore, the extra precautions required for handling and disposing of needles is obviated. It will be apparent from the detailed description provided herein that the present invention can provide for the elimination of nearly all needles used in the medical environment. With the use of the valve of the present invention, the need for all needles except those that are directly input into a patient is, advantageously, eliminated.

OPERATION

The valve 10 is used to provide a closed, patient access system for transferring a predetermined amount of medication from a remote source to the patient. The valve 10 is connected by the distal end to the patient, for example, a vein or artery in fluid communication with the valve. Blood fills the valve, but the seal 36d, for example, prevents any blood from leaking from the valve. The delivery end or nose 48 of the medical implement is inserted into the valve as depicted in FIG. 8, pushing the nose 48 against the seal to compress the seal sufficiently to allow the tip 32 of the spike 24 to pierce the seal and enter said delivery end. The predetermined amount of medication in its entirety may now be transferred through the nose 48 into the valve 10 and into the patient. Since the nose 48 and seal 36d engage in a manner so that the tip 32 of the spike element 24, upon

5,685,866

15

piercing the seal, meets the seal to avoid formation of any dead space at the interface between nose 48 and the seal surface 40b. Transfer directly through the valve 10 of essentially the entire predetermined amount of medication from the syringe 46 to the patient, so that essentially none of said predetermined amount is collected in any dead space in the valve, is accomplished with this invention. Upon withdrawing the nose 48 from the valve 10 the seal 36d returns to the decompressed state to close the valve and maintain while in said decompressed state a fluid tight seal even at high pressures and after repeated uses.

SCOPE OF THE INVENTION

The above presents a description of the best mode contemplated of carrying out the present invention, and of the manner and process of making and using it, in such full, clear, concise, and exact terms as to enable any person skilled in the art to which it pertains to make and use this invention. This invention is, however, susceptible to modifications and alternate constructions from that discussed above which are fully equivalent. Consequently, it is not the intention to limit this invention to the particular embodiments disclosed. On the contrary, the intention is to cover all modifications and alternate constructions coming within the spirit and scope of the invention as generally expressed by the following claims, which particularly point out and distinctly claim the subject matter of the invention.

I claim:

1. A medical valve comprising:
 - a body including wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end;
 - a spike having a tip, at least one hole located at or near said tip, and a passageway in communication with the hole that allows fluid to flow through said hole, said spike being seated within the cavity such that said tip is enclosed within the cavity; and
 - a resilient seal which is adapted to be moved distally in the cavity into a compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to a decompressed state upon removal of said delivery end from said opening, said seal in the decompressed state having a section which fills essentially completely a portion of the cavity adjacent said opening, said seal section bearing against said wall structure near said opening to seal said opening, and in the compressed state said seal section being located in the cavity distal of said opening, said seal comprising a series of O-ring elements stacked together and connected to form a unitary structure.
2. The medical valve of claim 1, wherein said O-ring elements have increasing diameters in the distal direction.
3. The medical valve of claim 1, wherein said seal in the decompressed state has a proximal end substantially flush with the proximal end of said cavity of said body.
4. The medical valve of claim 3, wherein said proximal end of said seal is substantially flat.

16

5. The medical valve of claim 1, wherein said seal is precut to form a tiny orifice therein, allowing the tip of said spike to pass through said seal easily upon compression of said seal in the distal direction.

6. The medical valve of claim 1, wherein said seal comprises a silicone polymer.

7. The medical valve of claim 1, wherein said medical valve further comprises a support member enabling said valve to be removably attached to a fluid dispenser.

8. The medical valve of claim 1, wherein said body contains at least one radial indentation.

9. A medical valve comprising:

a body including wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end, said body having a plurality of radial indentations in an interior wall thereof;

a spike having a tip, at least one hole located at or near said tip, and a passageway in communication with the hole that allows fluid to flow through said hole, said spike being seated within the cavity such that said tip is enclosed within the cavity; and

a resilient seal which is adapted to be moved distally in the cavity into a compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to a decompressed state upon removal of said delivery end from said opening, said seal in the decompressed state having a section which fills essentially completely a portion of the cavity adjacent said opening, said seal section bearing against said wall structure near said opening to seal said opening, and in the compressed state said seal section being located in the cavity distal of said opening.

10. The medical valve of claim 9, wherein said seal expands into said radial indentations upon distal compression of said seal.

11. The medical valve of claim 9, wherein said seal comprises a series of O-ring elements stacked together and connected to form a unitary structure.

12. The medical valve of claim 9, wherein said seal has a wall defined by a number of ringed wall sections which collapse and expand in accordion-like fashion.

13. The medical valve of claim 9, wherein said seal is precut to form a tiny orifice therein, allowing the tip of said spike to pass through said seal easily upon compression of said seal in the distal direction.

14. The medical valve of claim 9, wherein said seal comprises a silicone polymer.

15. The medical valve of claim 9, wherein said medical valve further comprises a support member enabling said valve to be removably attached to a fluid dispenser.

16. The medical valve of claim 9, wherein said seal in the decompressed state has a proximal end substantially flush with the proximal end of said cavity of said body.

17. The medical valve of claim 16, wherein said proximal end of said seal is substantially flat.

* * * * *

EXHIBIT B



US005873862A

United States Patent [19]
Lopez

[11] **Patent Number:** **5,873,862**
[45] **Date of Patent:** **Feb. 23, 1999**

[54] **MEDICAL VALVE AND METHOD OF USE**

WO 93/11828 5/1993 WIPO .

[75] Inventor: **George A. Lopez**, Corona del Mar, Calif.

[73] Assignee: **ICU Medical, Inc.**, San Clemente, Calif.

[21] Appl. No.: **841,408**

[22] Filed: **Apr. 22, 1997**

Related U.S. Application Data

[63] Continuation of Ser. No. 334,846, Nov. 4, 1994, Pat. No. 5,685,866, which is a continuation of Ser. No. 096,659, Jul. 23, 1993, which is a continuation-in-part of PCT/US92/10367 Dec. 1, 1992, which is a continuation-in-part of Ser. No. 813,073, Dec. 18, 1991, abandoned.

[51] **Int. Cl.⁶** **A61M 5/00**

[52] **U.S. Cl.** **604/249; 604/33; 604/246; 604/283**

[58] **Field of Search** 604/30, 33, 246, 604/249, 283

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 321,250 10/1991 Jepson et al. .
D. 321,251 10/1991 Jepson et al. .
1,578,517 3/1926 Hein .
2,289,677 7/1942 Perelson .
2,847,995 8/1958 Adams .
3,134,380 5/1964 Armao .
3,135,261 6/1964 Carroll .

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

1105959 7/1981 Canada .
0 114 677 A2 8/1984 European Pat. Off. .
0 237 321 3/1987 European Pat. Off. .
0 240 987 A2 10/1987 European Pat. Off. .
0 309 771 A1 9/1988 European Pat. Off. .
0 446 463 A1 12/1990 European Pat. Off. .
84 25 197 2 9/1985 Germany .
WO 86/01712 3/1986 WIPO .
WO 86/03415 6/1986 WIPO .

OTHER PUBLICATIONS

NITA I.V. Standards of Practice, pp. 71, 72 and Exhibit A. showing Nutri-Flor Product, vol. 5, Jan.-Feb. 1982.

Baxter Product Brochure, "Closed Draining Bag", 2 pages.

Baxter Product Brochure, "Urine Sampling Unit", 2 pages.

Travenol Laboratories, Inc. Product ad, "Mini-Bag Under-fill Vialflex Containers", 3 pages.

NITA, vol. 7, No. 2 Mar./Apr. 1984, 6 pages.

Travenol Ad, "The Continu-Flo Administration System", 4 pages.

American Journal of Hospital Pharmacy, vol. 26, Jan. 1969, 12 pages.

American Journal of Hospital Pharmacy, vol. 36, Nov. 1979, 7 pages.

American Society of Hospital Pharmacists "Evaluation of Piggyback Administration Sets", vol. 34, Dec. 1977, pp. 1315-1323.

Primary Examiner—Wynn Wood Coggins


Assistant Examiner—Cris L. Rodriguez

Attorney, Agent, or Firm—Knobbe, Martens, Olson & Bear, LLP

[57] **ABSTRACT**

A closed system, needleless valve device includes a generally tubular body defining an internal cavity. On the proximal end of the body there is an opening which is preferably sufficiently large to receive an ANSI standard tip of a medical implement. The distal end of the body has a generally tubular skirt. The valve also includes a hollow spike having a closed tip. The spike includes at least one longitudinal 18-gauge hole located distal the tip, and is seated inside the cavity such that the tip is below the proximal end of the body. An annular support cuff is connected to the spike which seals off a portion of the cavity of the body such that an upper cavity containing the tip is defined. The valve also includes a plastic, resilient silicone seal which fills the upper cavity and opening and covers the tip of the spike so as to present a flush surface. An adaptor enables the valve to be attached to a resealable container.

5 Claims, 19 Drawing Sheets

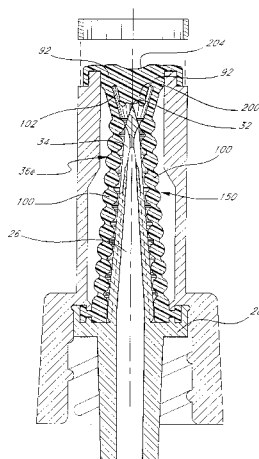

5,873,862

Page 2

U.S. PATENT DOCUMENTS


3,354,881	11/1967	Bloch .	4,706,487	11/1987	Bandou et al. .
3,648,648	3/1972	Barnwell, et al. .	4,725,267	2/1988	Vaillancourt .
3,852,385	12/1974	Huggins .	4,752,292	6/1988	Lopez et al. .
3,974,832	8/1976	Kruck .	4,775,369	10/1988	Schwartz .
3,976,063	8/1976	Henneman et al. .	4,781,702	11/1988	Herrli .
3,986,508	10/1976	Barrington .	4,810,241	3/1989	Rogers .
4,019,512	4/1977	Tenczar .	4,826,500	5/1989	Rautsola .
4,076,285	2/1978	Martinez .	4,846,809	7/1989	Sims .
4,079,738	3/1978	Dunn et al. .	4,874,377	10/1989	Newgard et al. .
4,080,965	3/1978	Phillips .	4,950,260	8/1990	Bonaldo .
4,121,585	10/1978	Becker, Jr. .	4,964,855	10/1990	Todd et al. .
4,128,098	12/1978	Bloom et al. .	4,969,883	11/1990	Gilbert et al. .
4,161,949	7/1979	Thanawalla .	4,981,469	1/1991	Whitehouse et al. .
4,187,846	2/1980	Lolachi et al. .	4,998,713	3/1991	Vaillancourt .
4,219,912	9/1980	Adams .	4,998,921	3/1991	Vickroy et al. .
4,328,802	5/1982	Curley et al. .	4,998,927	3/1991	Vaillancourt .
4,334,551	6/1982	Pfister .	5,069,225	12/1991	Okamura .
4,338,933	7/1982	Bayard et al. .	5,100,394	3/1992	Dudar et al. .
4,411,662	10/1983	Pearson .	5,122,123	6/1992	Vaillancourt .
4,417,890	11/1983	Dennehey et al. .	5,135,489	8/1992	Jepson et al. .
4,432,759	2/1984	Gross et al. .	5,154,703	10/1992	Bonaldo .
4,432,765	2/1984	Oscarsson .	5,158,554	10/1992	Jepson et al. .
4,439,193	3/1984	Larkin .	5,167,642	12/1992	Fowles .
4,457,749	7/1984	Bellotti et al. .	5,167,647	12/1992	Wijkamp et al. .
4,508,367	4/1985	Oreopoulos et al. .	5,167,648	12/1992	Jepson et al. .
4,511,359	4/1985	Vaillancourt .	5,171,234	12/1992	Jepson et al. .
4,512,766	4/1985	Vaillancourt .	5,188,620	2/1993	Jepson et al. .
4,592,356	6/1986	Gutierrez .	5,211,638	5/1993	Dudar et al. .
4,610,469	9/1986	Wolff-Mooij .	5,273,533	12/1993	Bonaldo .
4,617,012	10/1986	Vaillancourt .	5,290,254	3/1994	Vaillancourt .
4,645,494	2/1987	Lee et al. .	5,344,414	9/1994	Lopez et al. .
4,673,400	6/1987	Martin .	5,401,245	3/1995	Haining .
			5,411,499	5/1995	Dudar et al. .

U.S. Patent

Feb. 23, 1999

Sheet 1 of 19

5,873,862

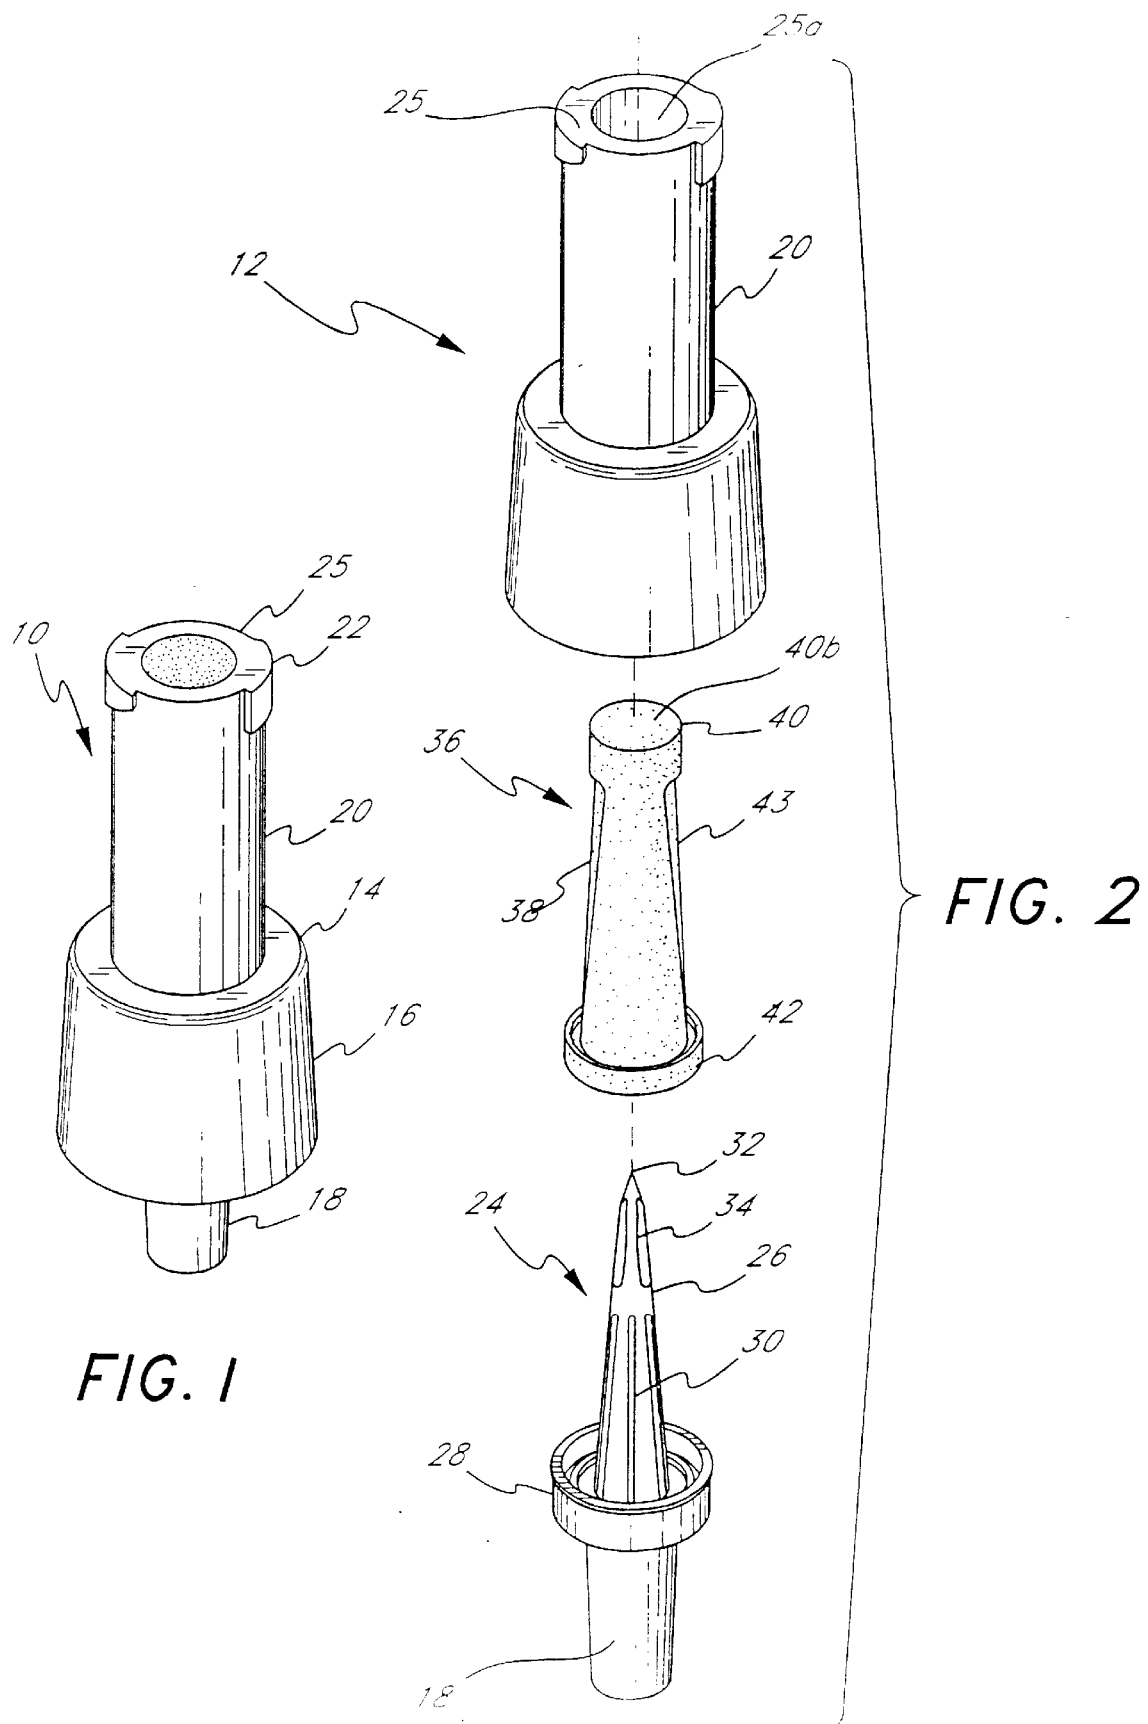

U.S. Patent

Feb. 23, 1999

Sheet 3 of 19

5,873,862

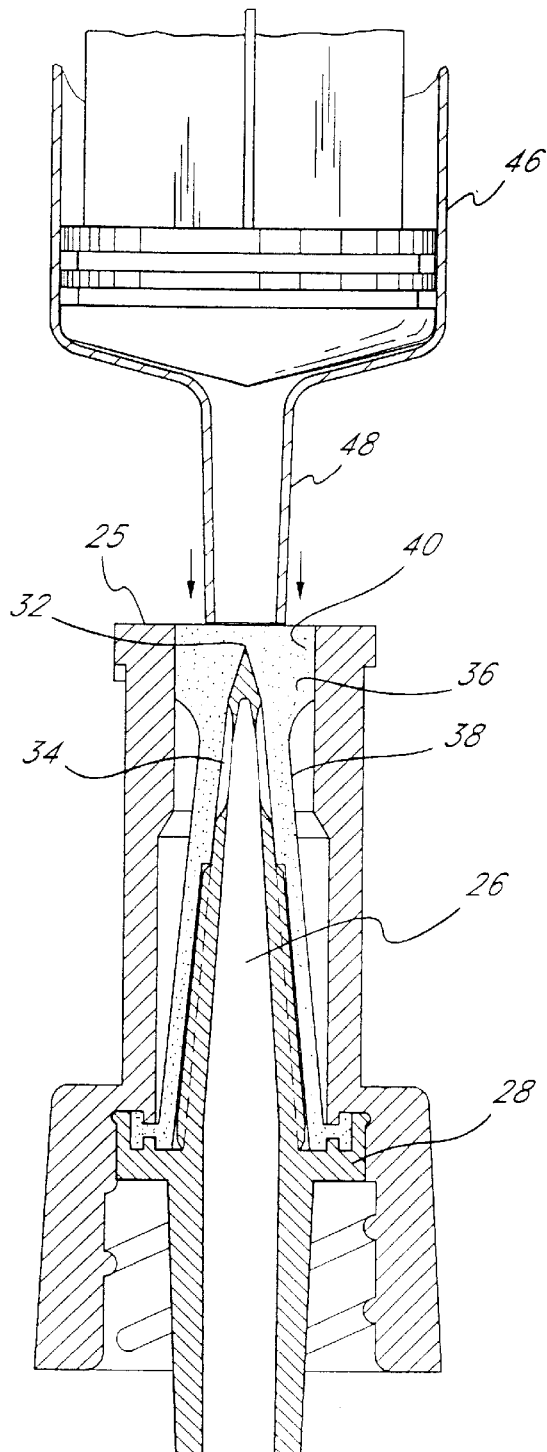


FIG. 4

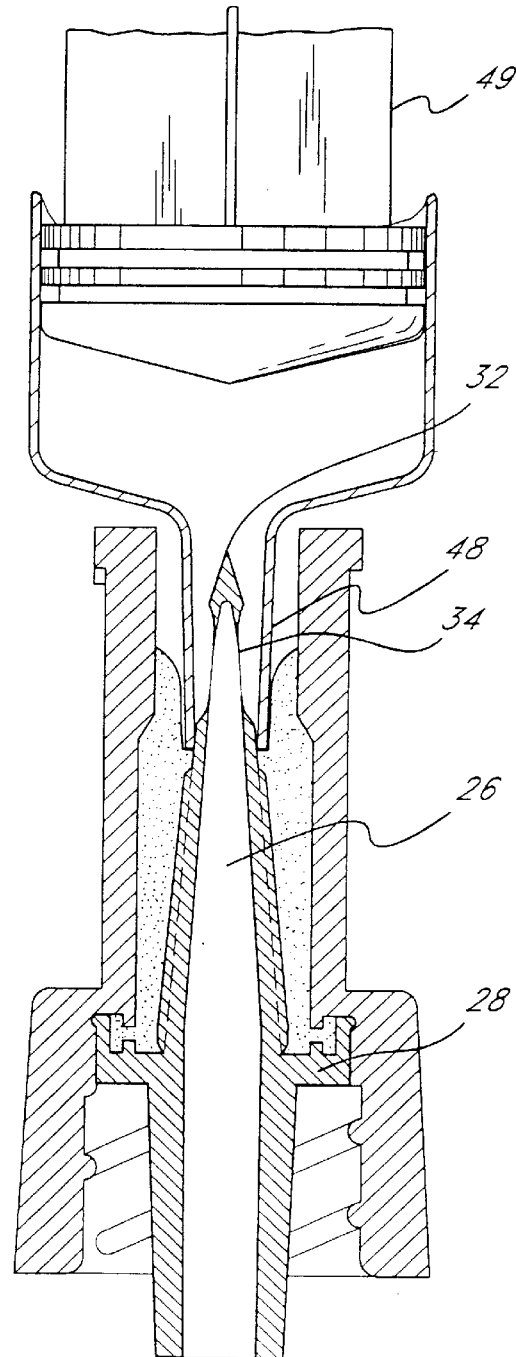


FIG. 5

U.S. Patent

Feb. 23, 1999

Sheet 4 of 19

5,873,862

FIG. 6



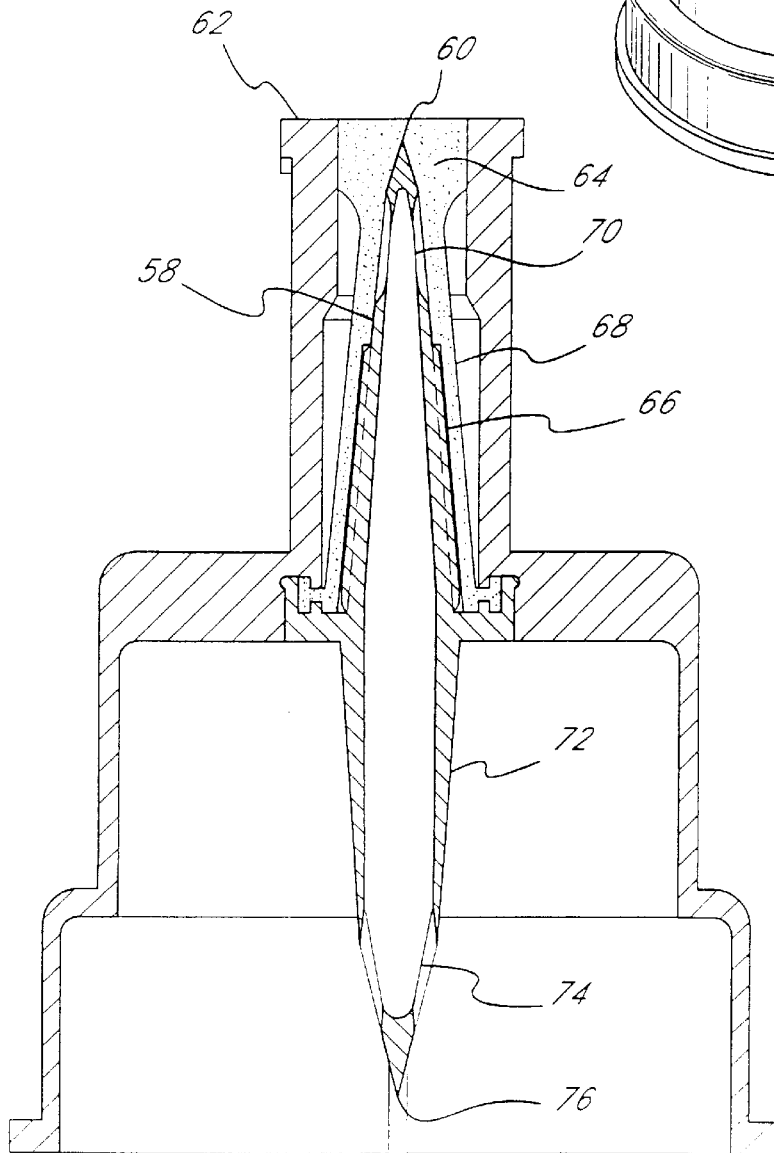


FIG. 7

FIG. 8

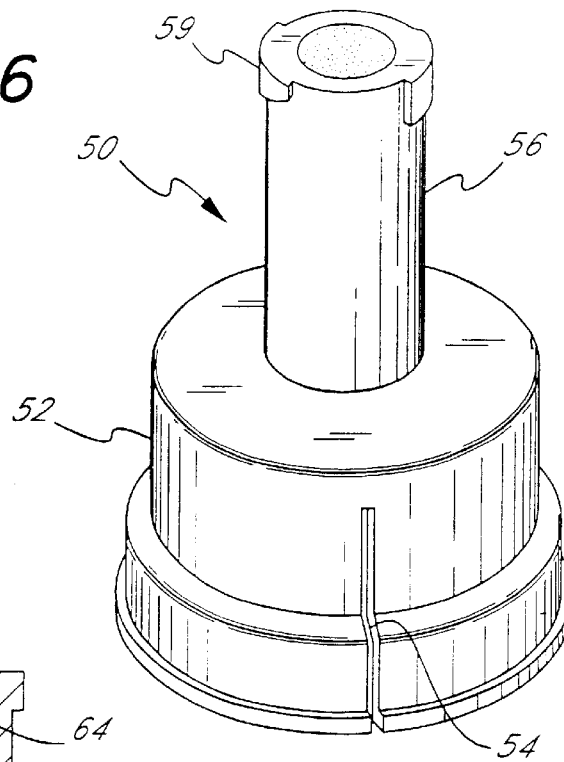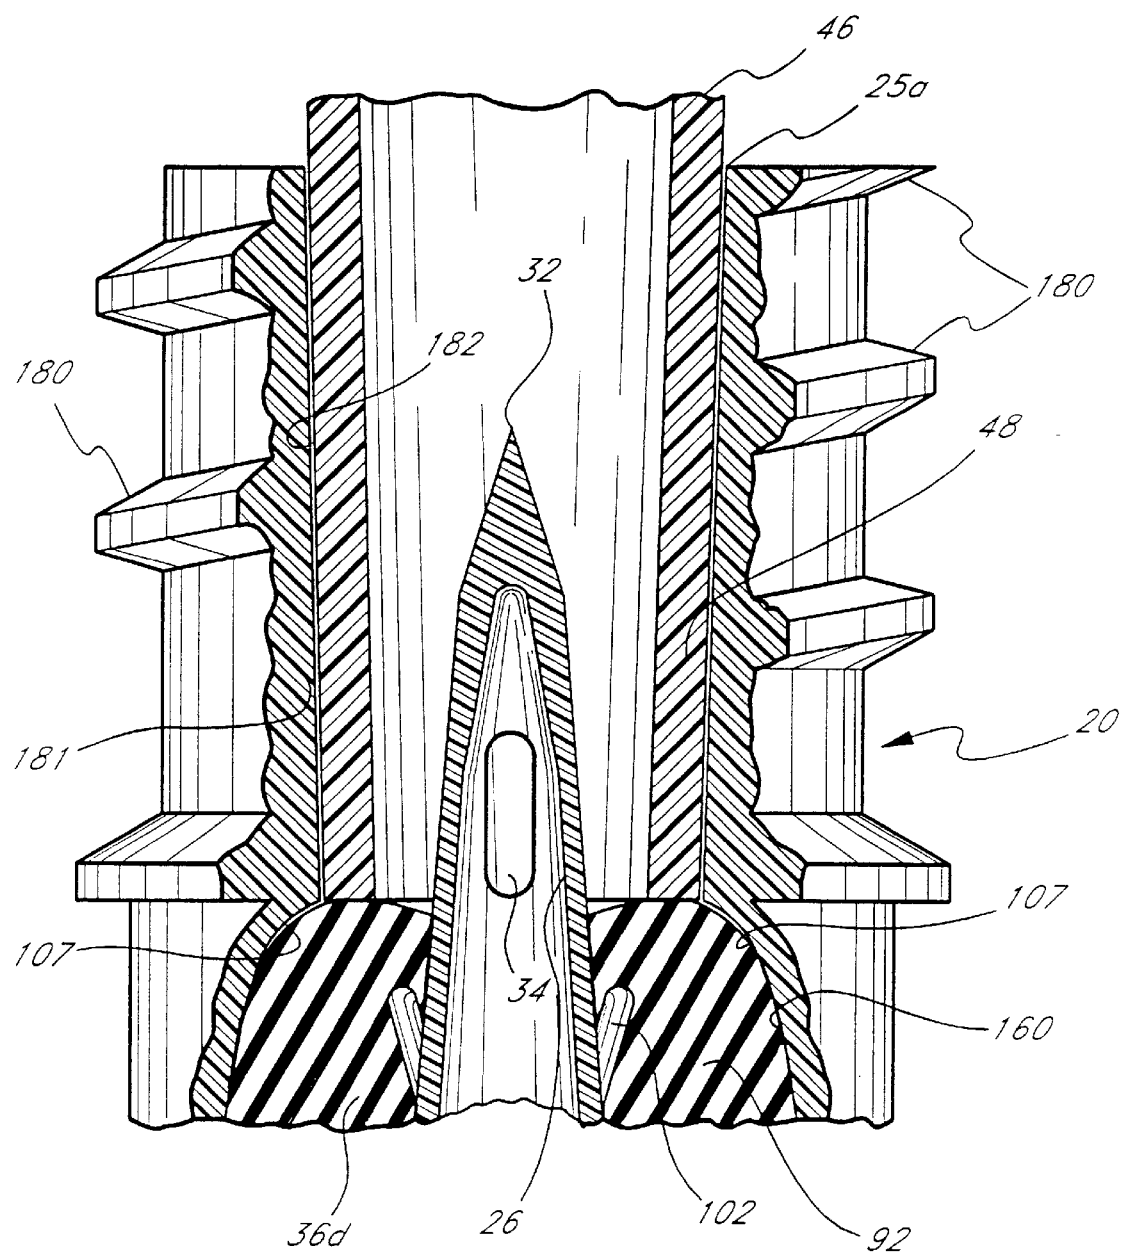

U.S. Patent

Feb. 23, 1999

Sheet 6 of 19

5,873,862

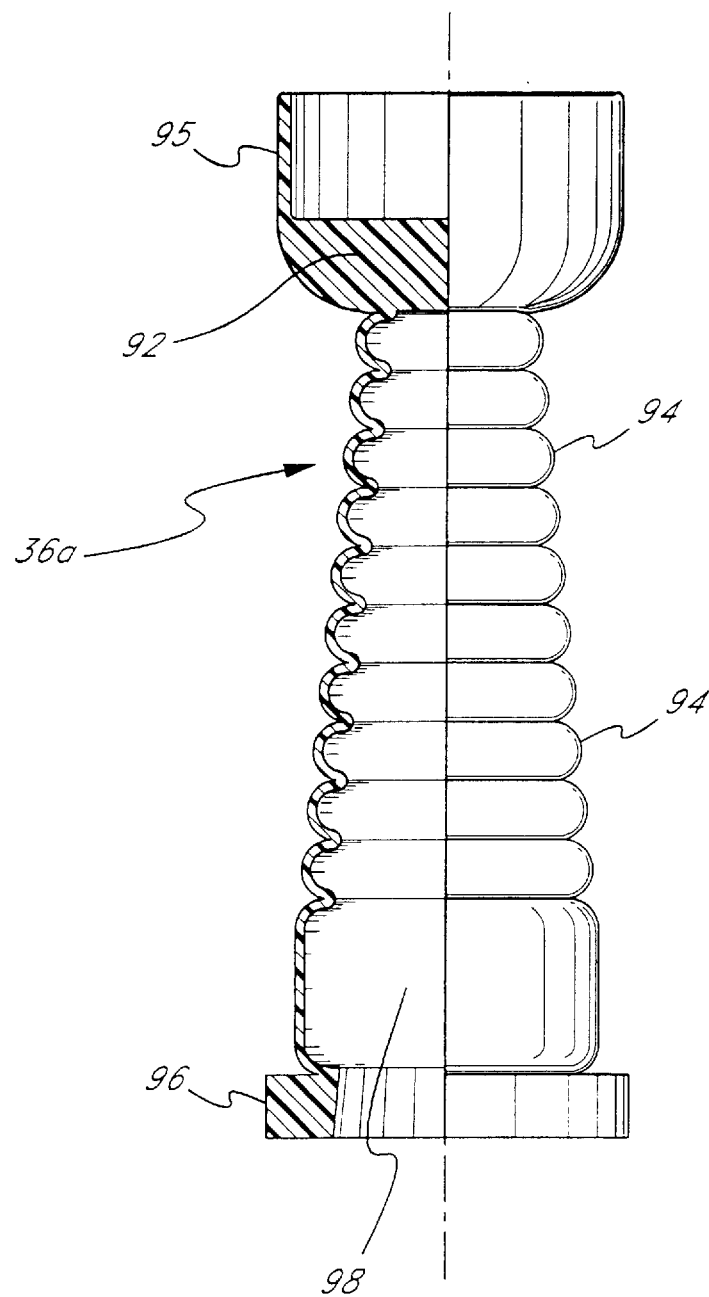


FIG. 9

U.S. Patent

Feb. 23, 1999

Sheet 7 of 19

5,873,862

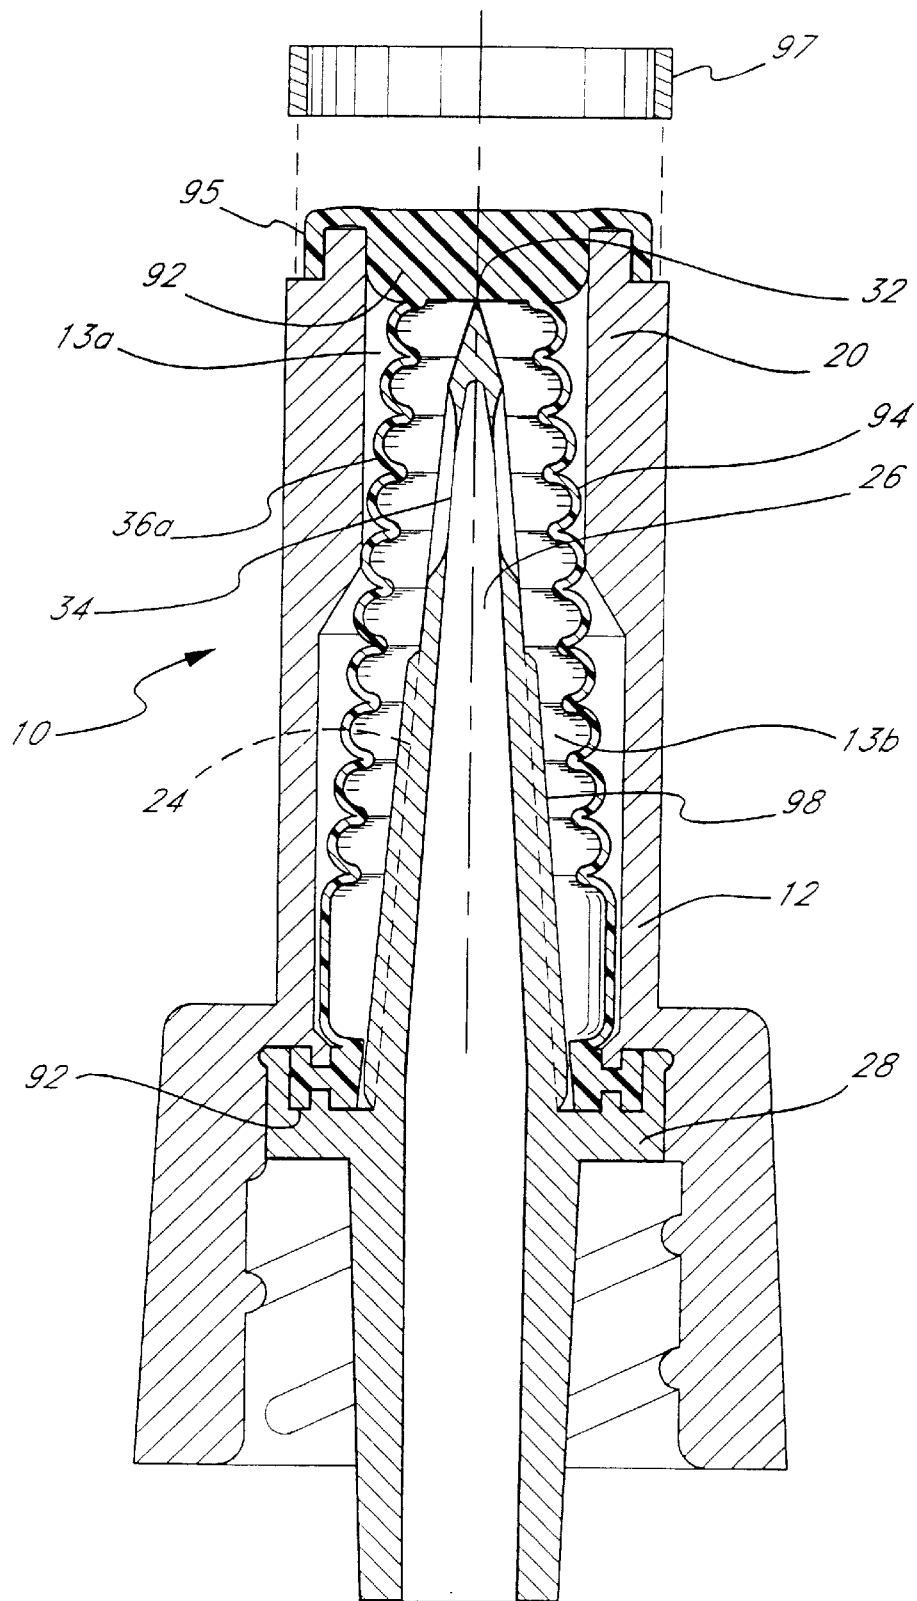


FIG. 10

U.S. Patent

Feb. 23, 1999

Sheet 8 of 19

5,873,862

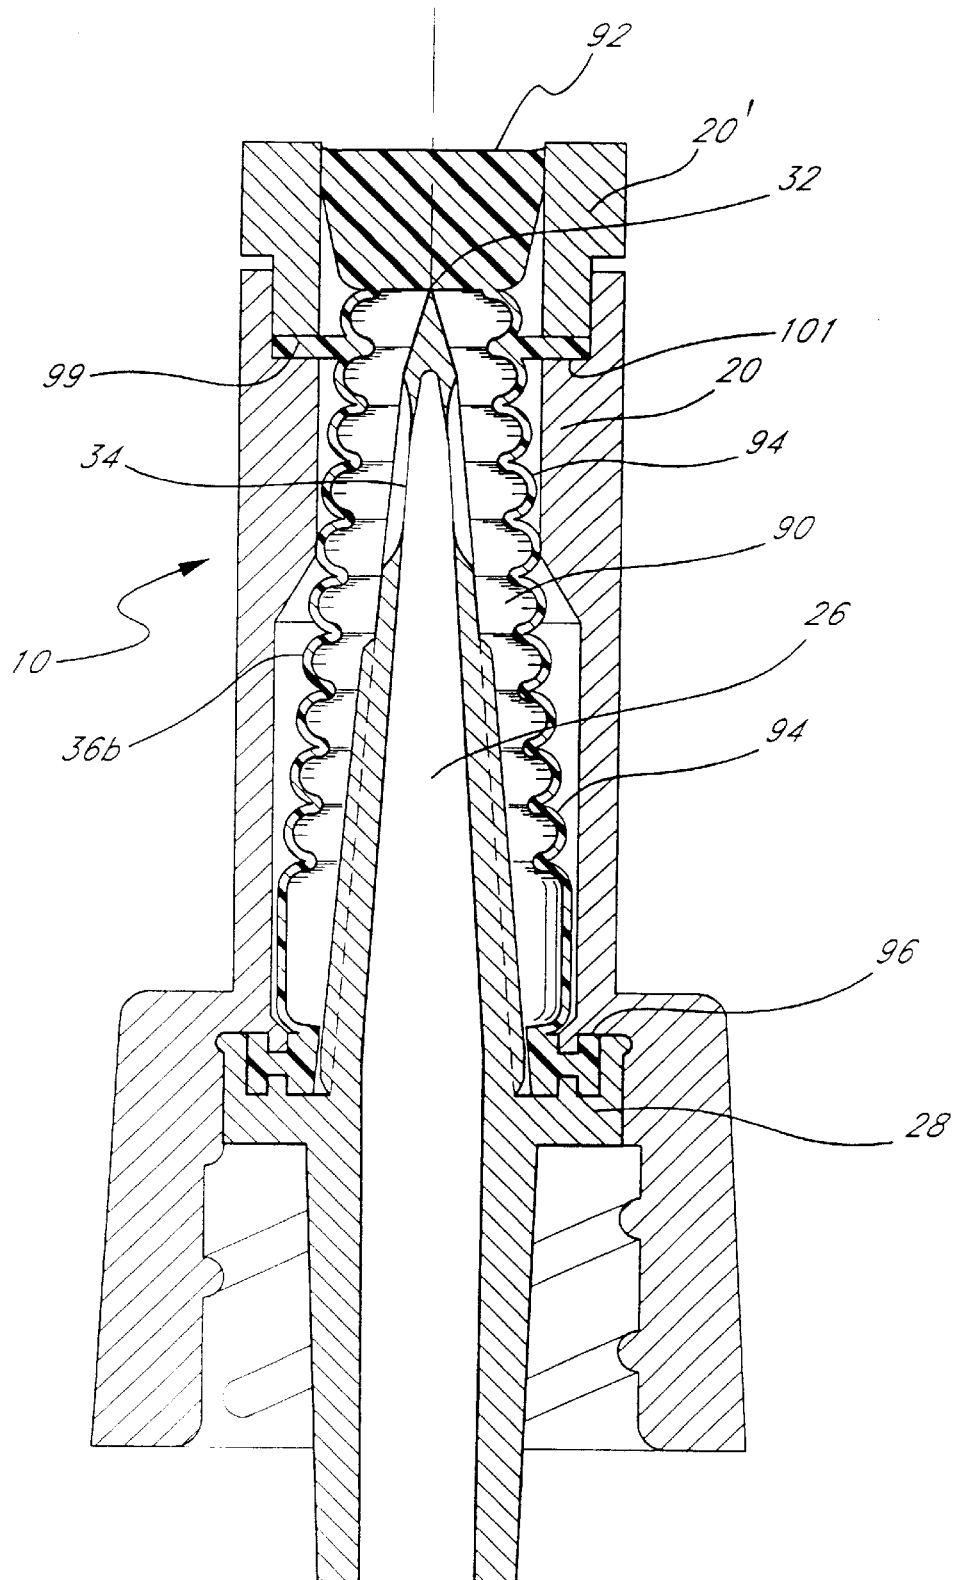


FIG. 11

U.S. Patent

Feb. 23, 1999

Sheet 9 of 19

5,873,862

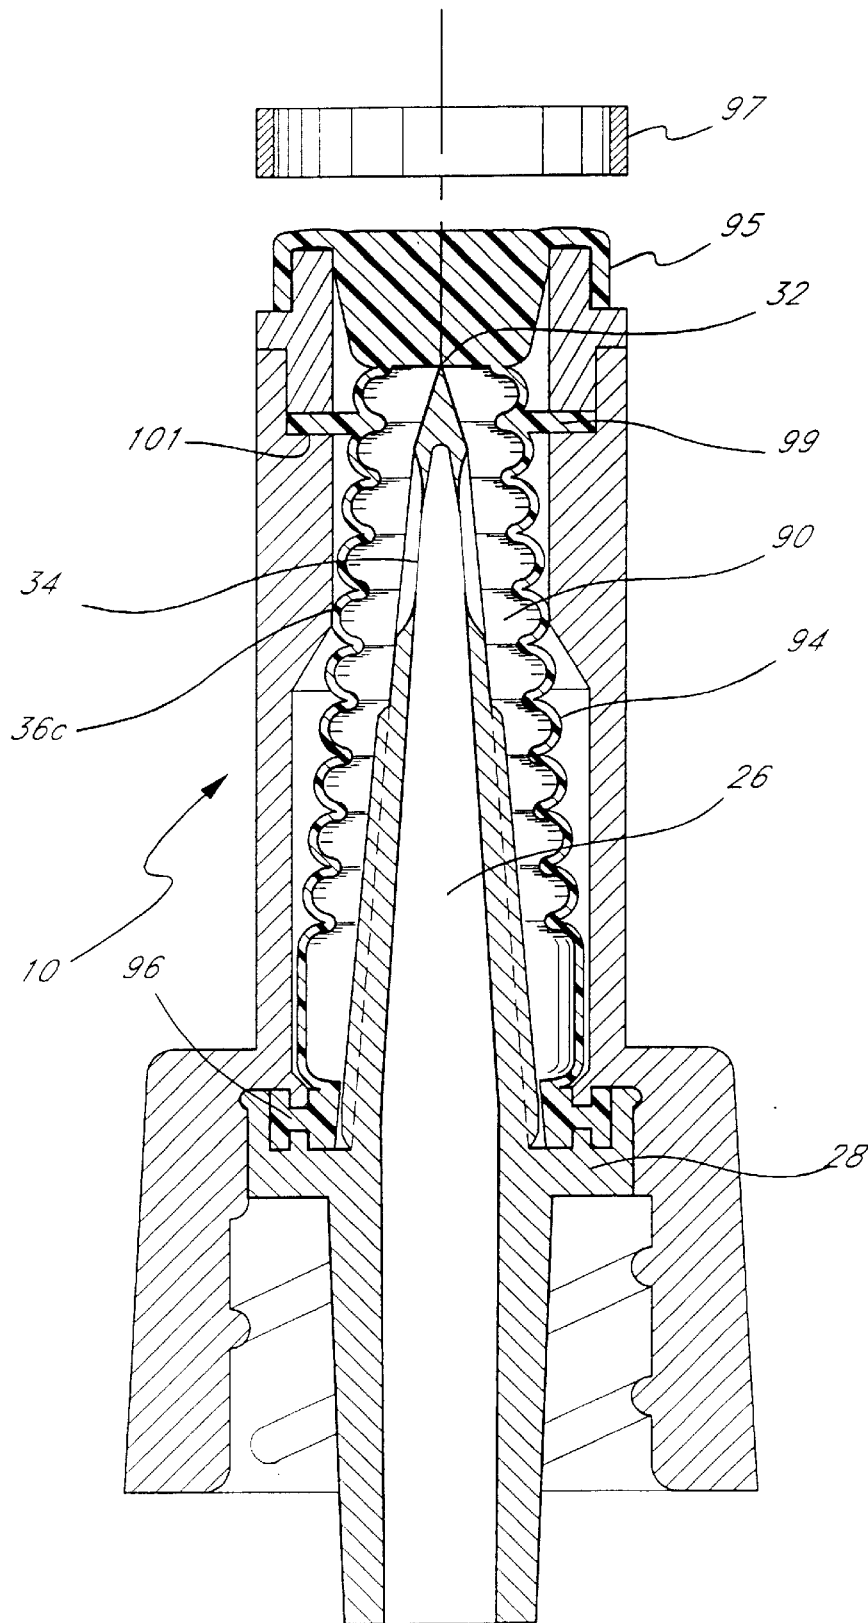


FIG. 12

U.S. Patent

Feb. 23, 1999

Sheet 10 of 19

5,873,862

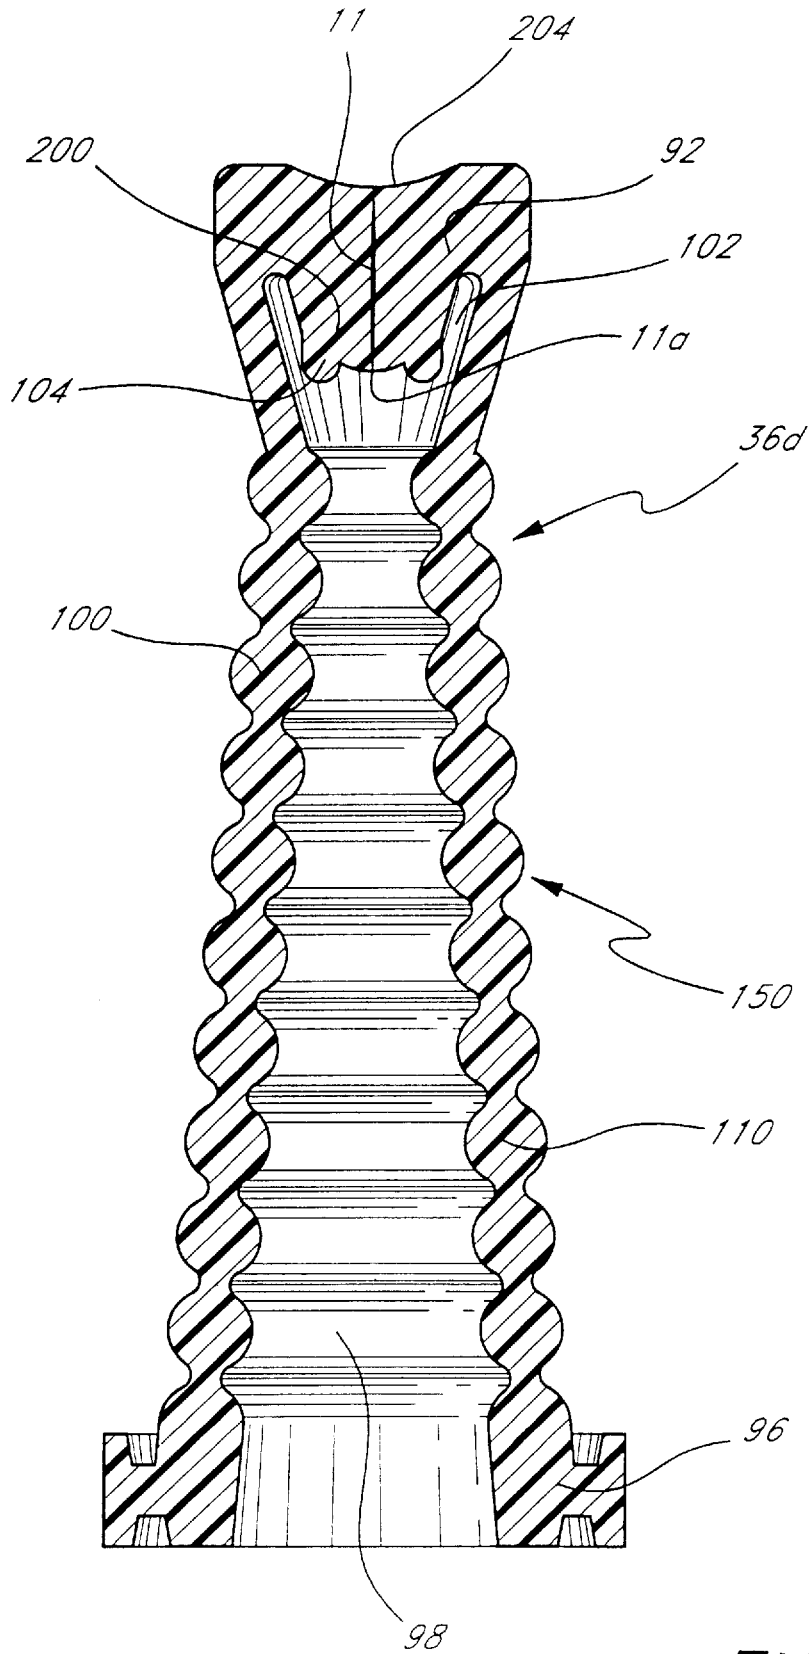


FIG. 13

U.S. Patent

Feb. 23, 1999

Sheet 11 of 19

5,873,862

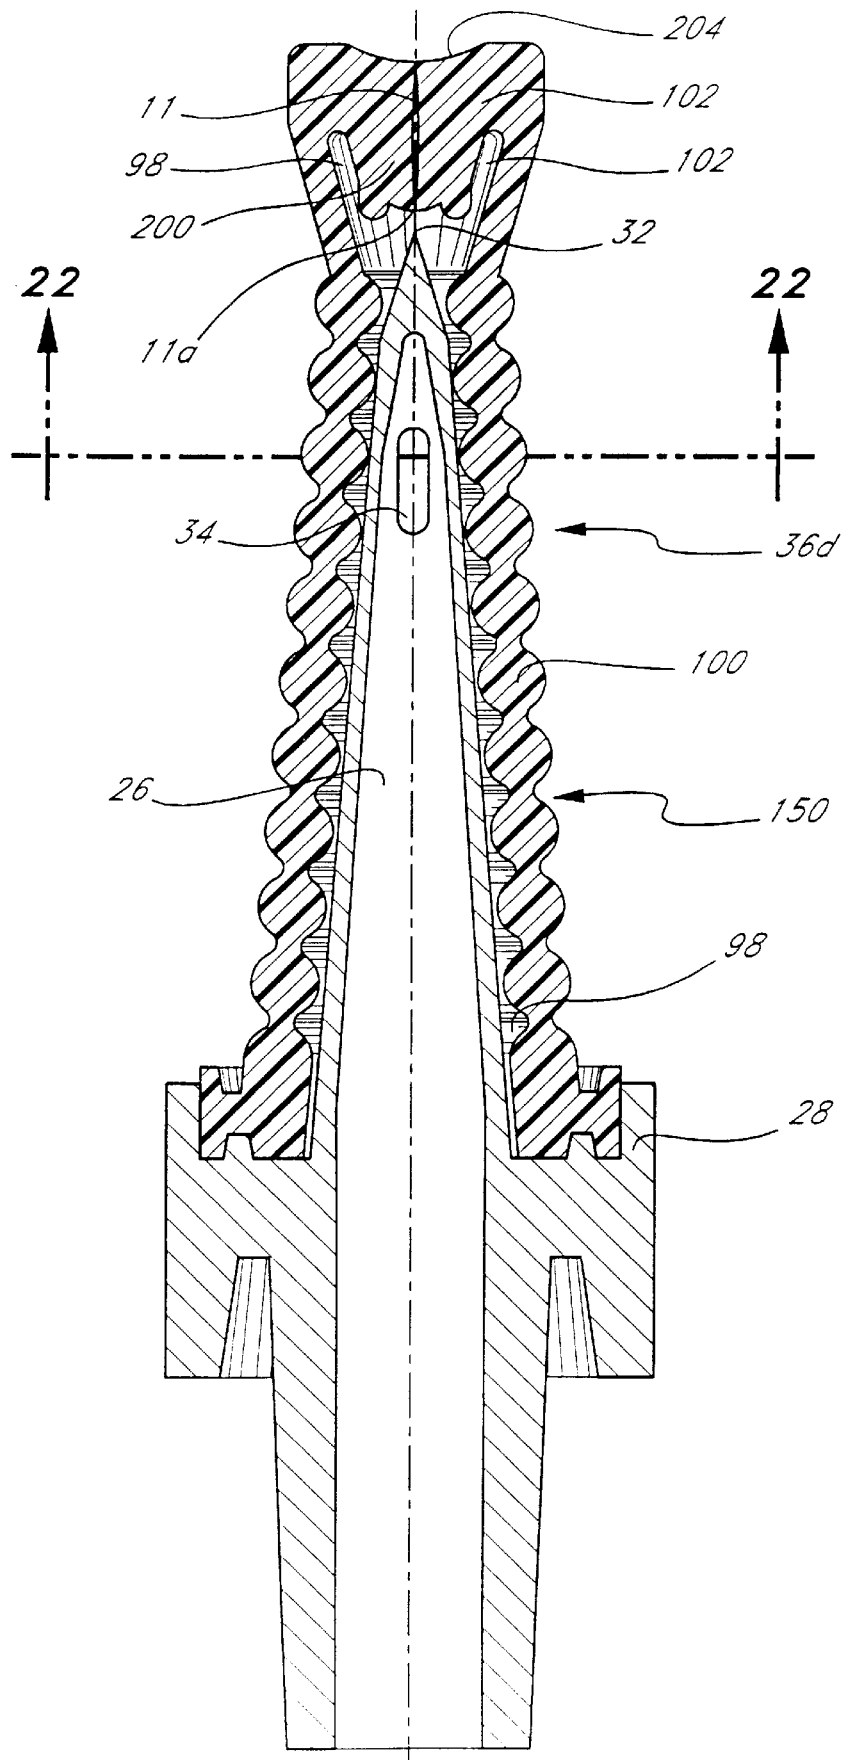


FIG. 14

U.S. Patent

Feb. 23, 1999

Sheet 12 of 19

5,873,862

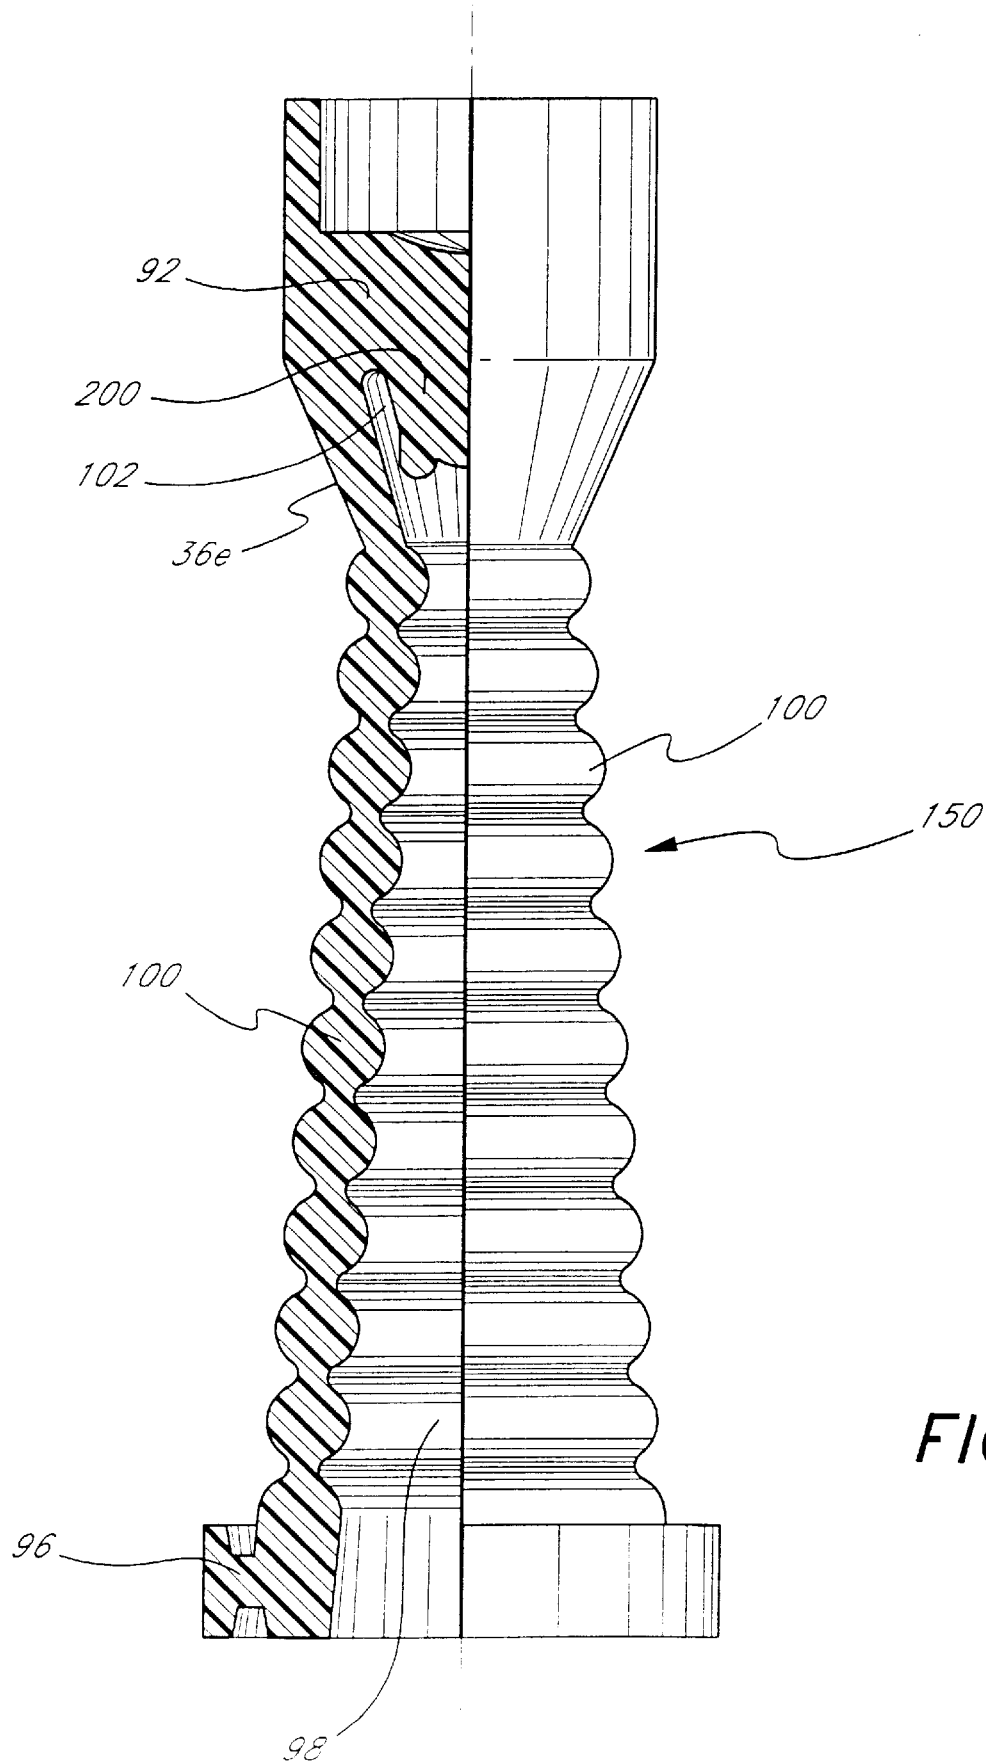


FIG. 15

U.S. Patent

Feb. 23, 1999

Sheet 13 of 19

5,873,862

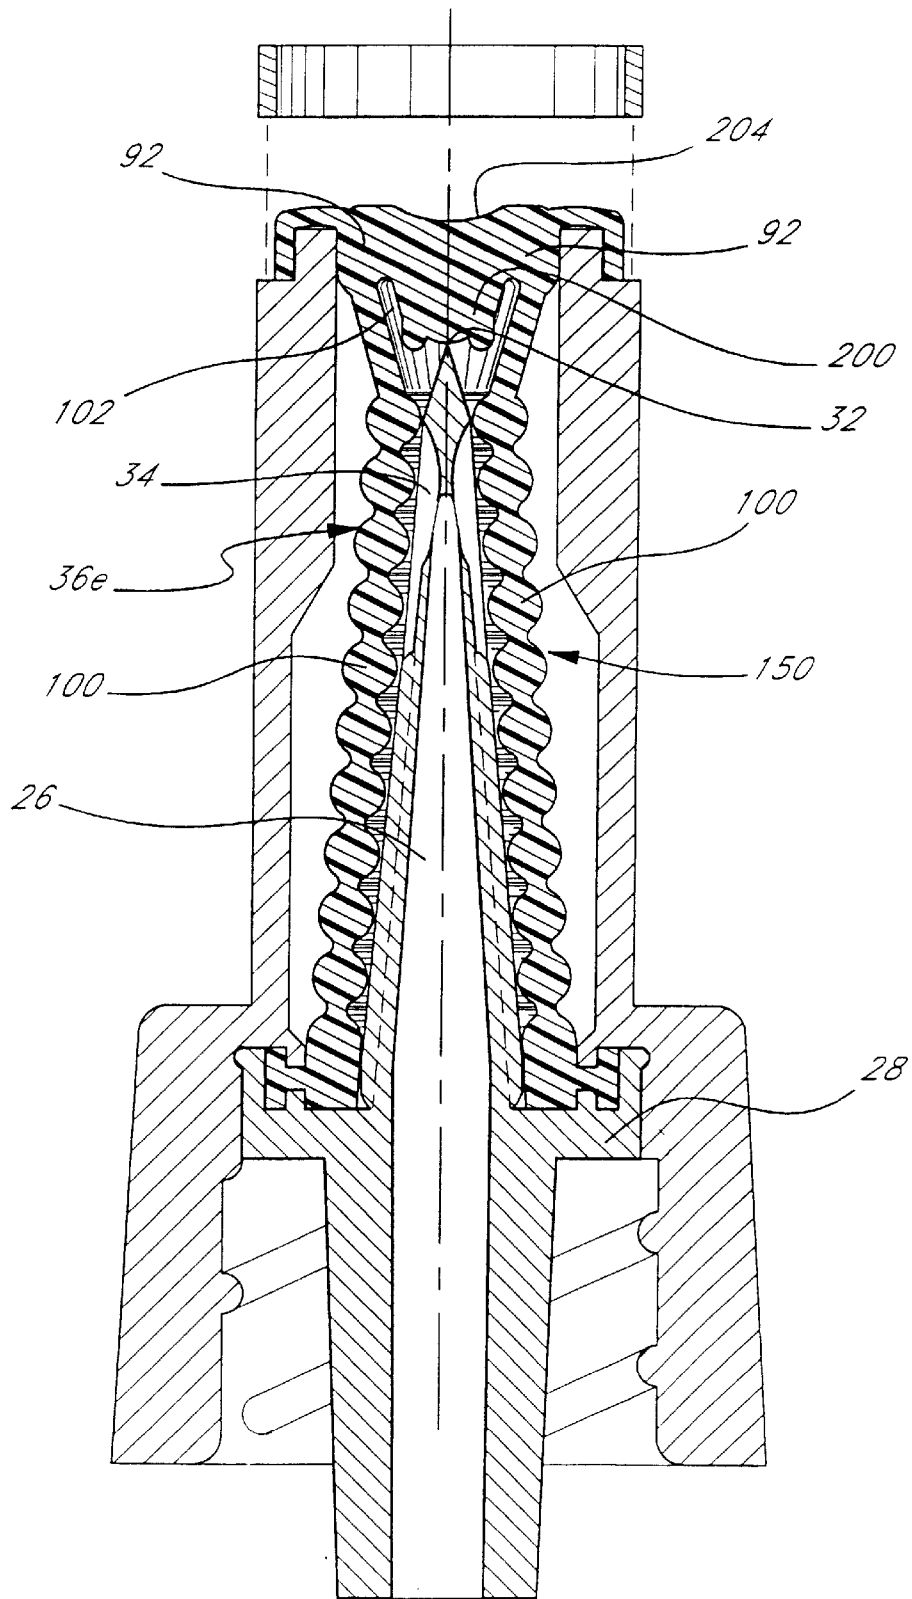


FIG. 16

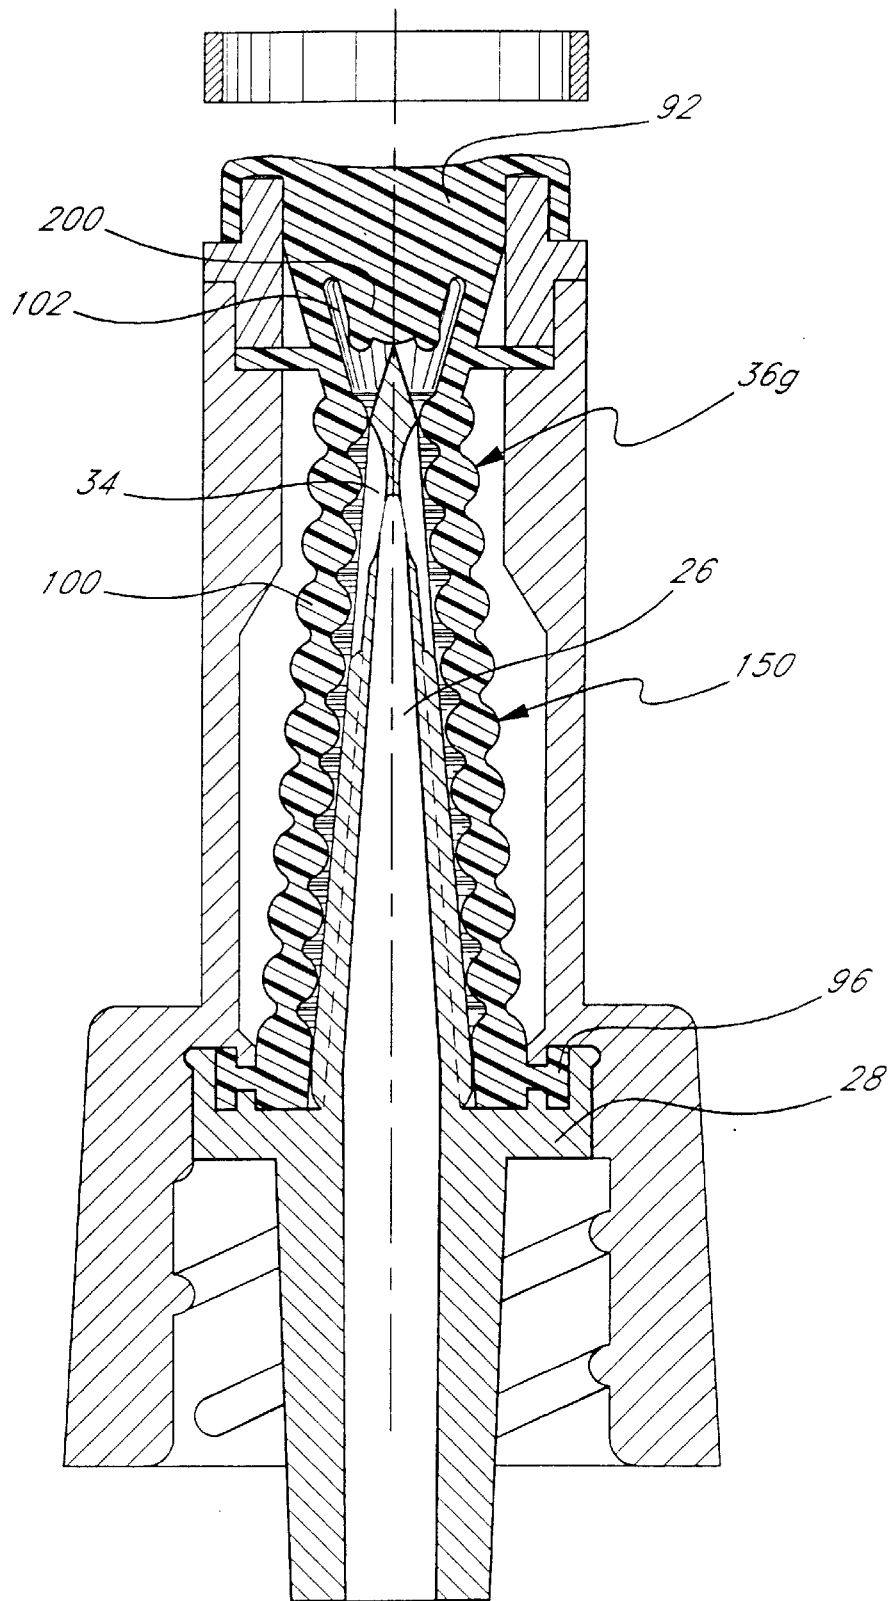


FIG. 18


U.S. Patent

Feb. 23, 1999

Sheet 16 of 19

5,873,862

FIG. 19

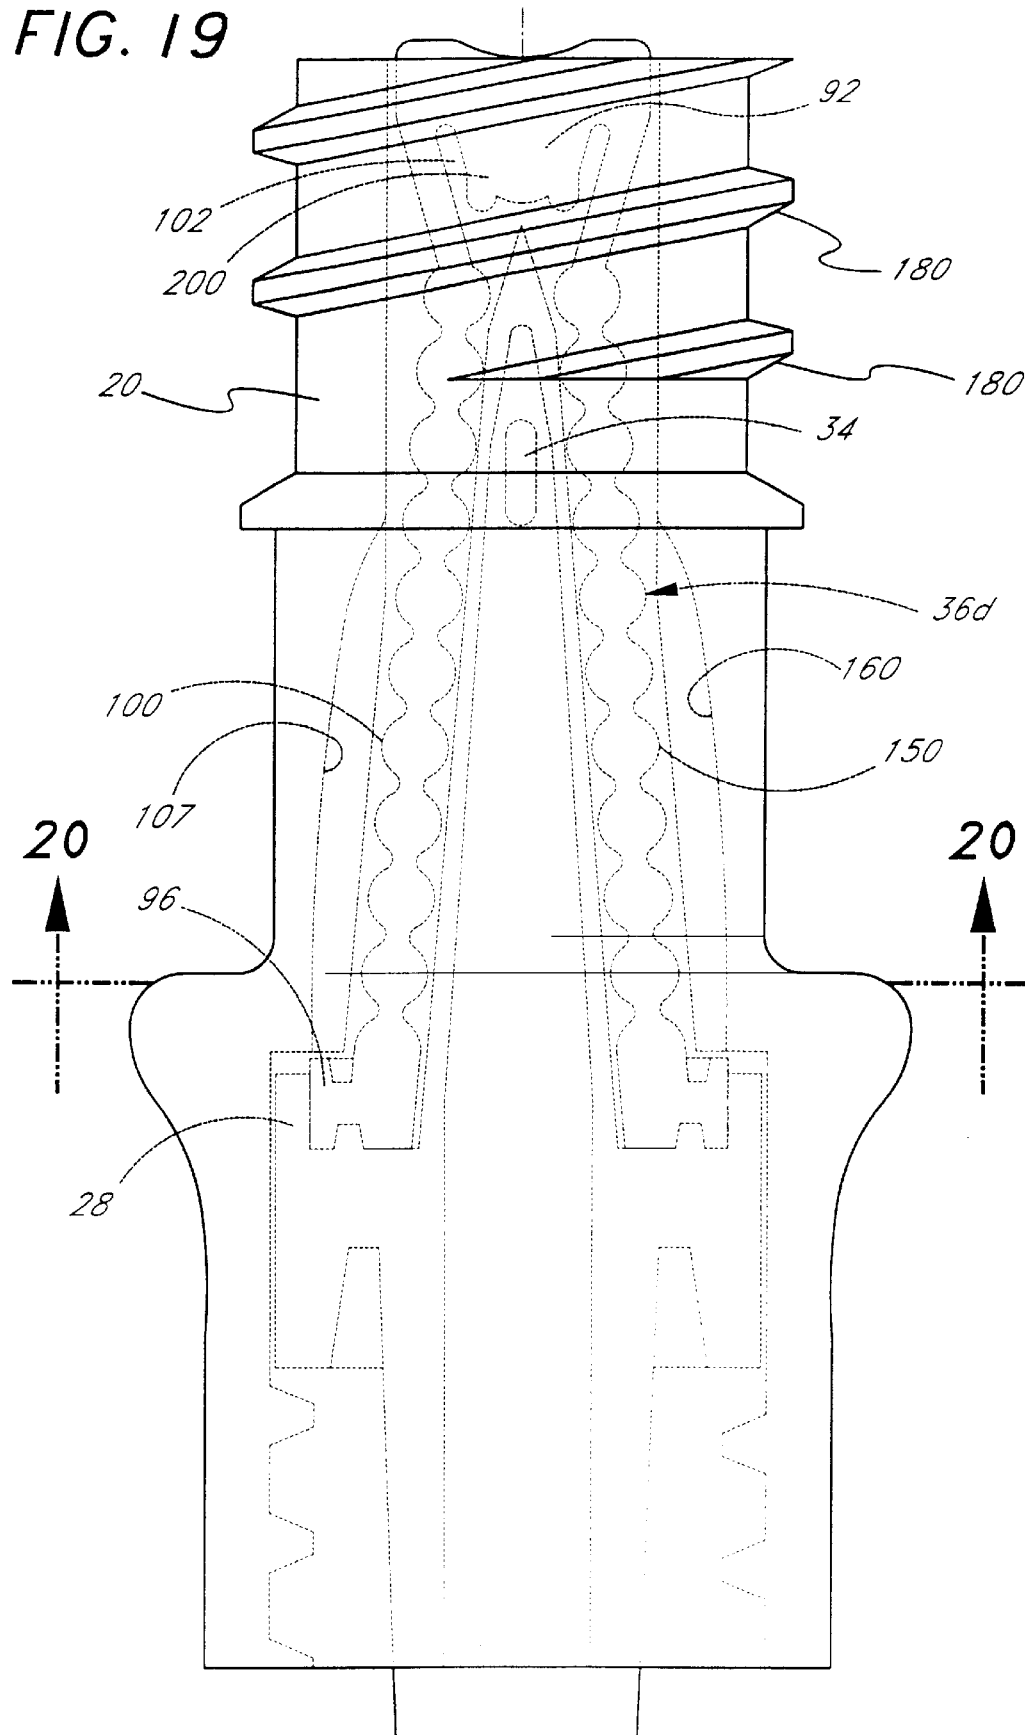

U.S. Patent

Feb. 23, 1999

Sheet 17 of 19

5,873,862

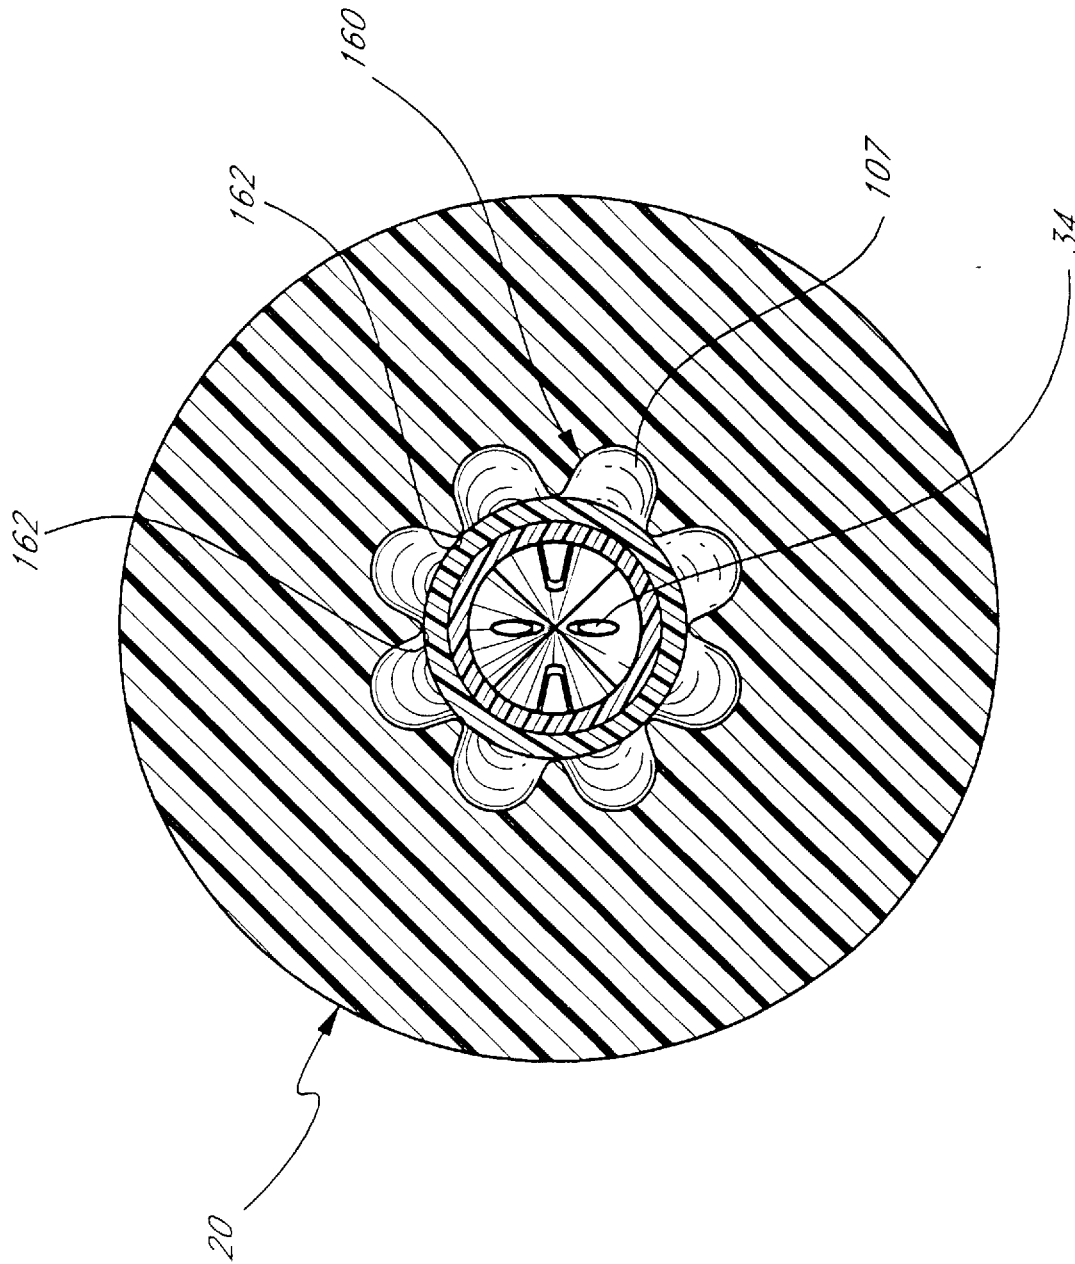


FIG. 20


U.S. Patent

Feb. 23, 1999

Sheet 18 of 19

5,873,862

FIG. 21

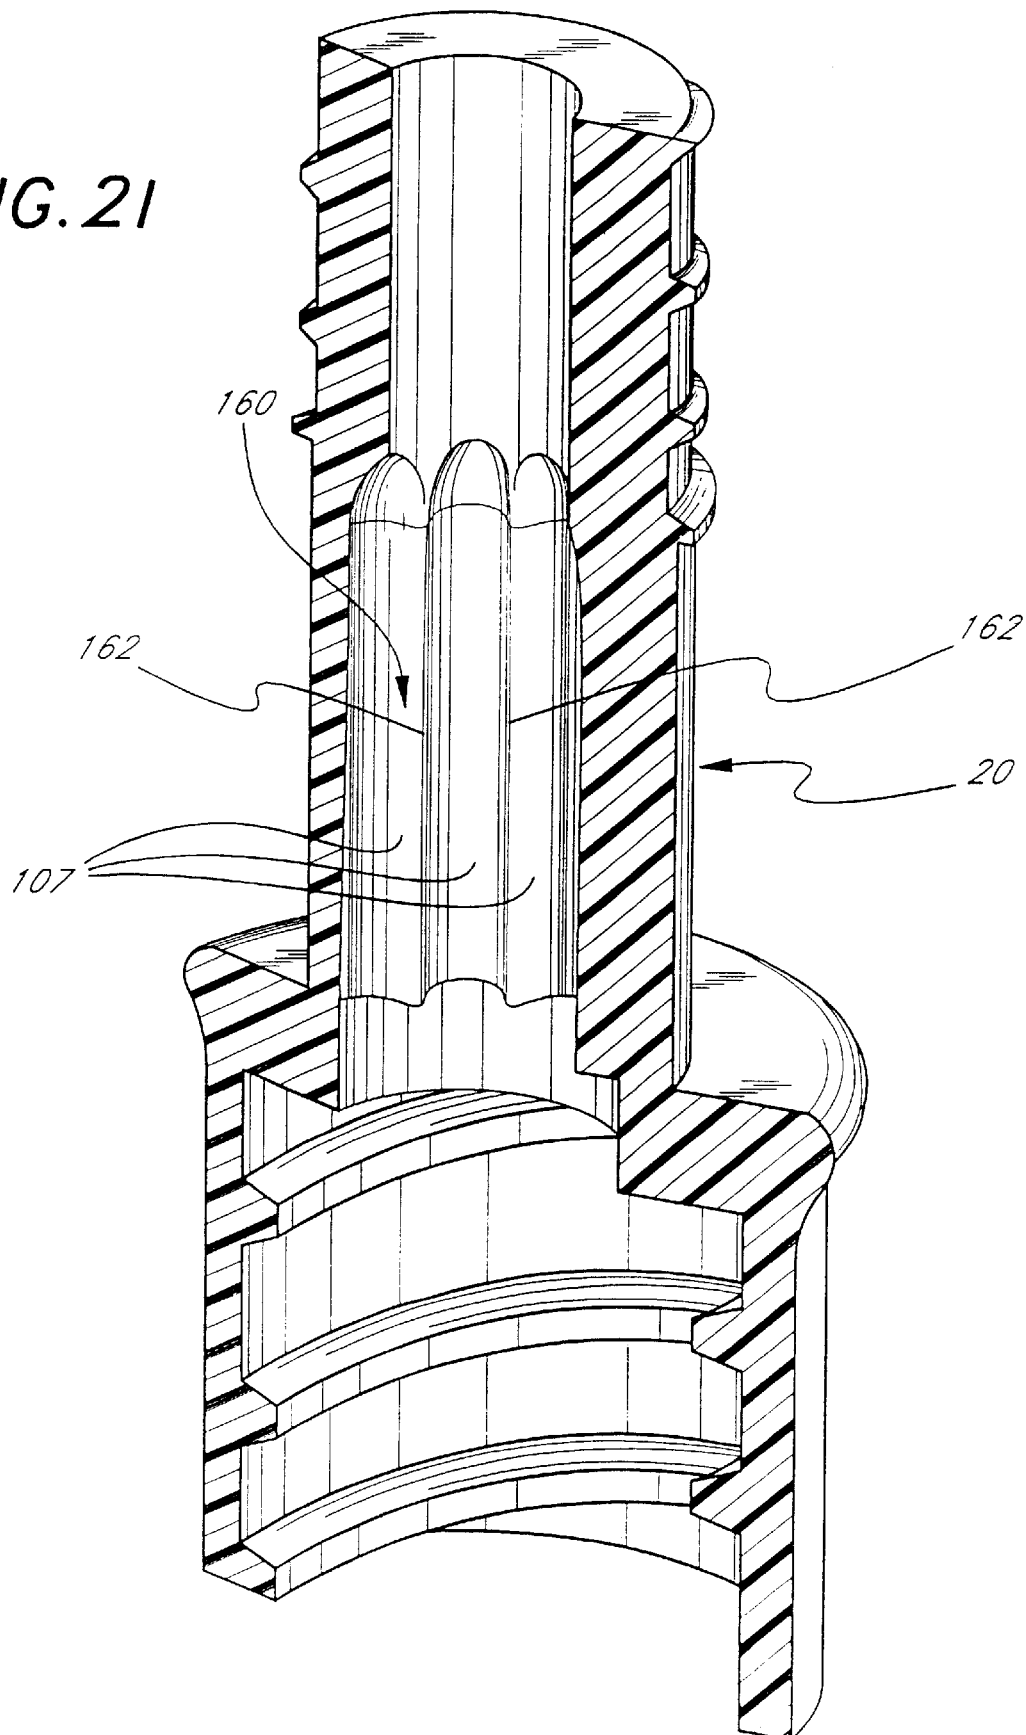

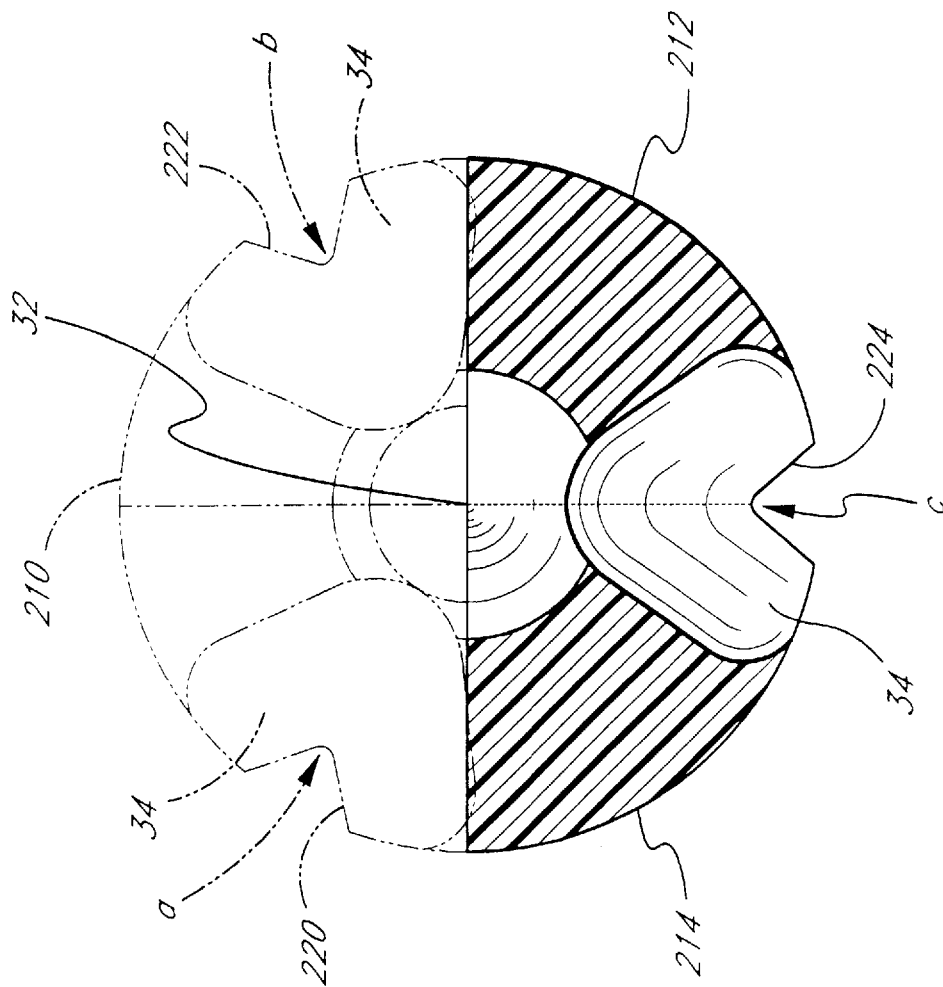


FIG. 22

5,873,862

1

MEDICAL VALVE AND METHOD OF USE

This application is a continuation of U.S. patent application Ser. No. 08,334,846, filed Nov. 4, 1994, now U.S. Pat. No. 5,685,866 which is a continuation of U.S. patent application Ser. No. 08,096,659 filed Jul. 23, 1993, which is a continuation-in-part of PCT Application Ser. No. PCT/US92/10367 filed Dec. 1, 1992, now abandoned, which is a continuation-in-part of U.S. patent application Ser. No. 07,813,073 filed Dec. 18, 1991, now abandoned.

BACKGROUND OF THE INVENTION**1. Field of The Invention**

This invention relates to a closed, patient access system which automatically reseals after administering medication using a standard medical implement that directly connects with the system without the need of any intermediary needles, caps; or adaptors. A two-way valve eliminating dead space is used which includes a seal which, upon being compressed by the medical implement, is pierced to open the valve and reseals upon being decompressed, maintaining a fluid tight seal even at high pressures and after repeated uses.

2. Background Discussion

The manipulation of fluids for parenteral administration in hospital and medical settings routinely involves the use of connectors and adaptors for facilitating the movement of fluids between two points. Most fluid connectors and adaptors employ needles to pierce a septum covering sterile tubing or to pierce the septum of a medicament container of fluid. Fluid then passes from the container or fluid filled tubing into a syringe or second set of tubing. These connectors and adaptors often have mechanical or moving parts. Since the ready passage of fluids through the connectors and adaptors is often critical to patient survival, it is imperative that the connectors and adaptors function reliably and repeatedly. Adaptors and connectors that malfunction during use may be life-threatening. The more mechanical or moving parts such as springs and diaphragms, the more likely that they will function improperly. Improper functioning can result in the introduction of air embolisms into a patient. Thus, the fewer the mechanical parts, the more these connectors can be relied on and the better they will be accepted by the medical community.

Many connectors or valves, especially those employing several mechanical components, have a relatively high volume of fluid space within them. This "dead space" within the device prevents accurate introduction of precise fluid volumes and provides an opportunity for contamination upon disconnection of the device. Connectors and adaptors often include valves that permit or interrupt the flow of fluid along the course of fluid travel. Several of those commonly in use employ metal needles to puncture sterile seals. Such connectors are generally designed to accommodate fluid flow in one direction. This means that the fluid line must have connectors and tube aligned in complementary directions. These connectors often require further manipulation if, for example, the valve is inadvertently assembled in a direction that will not facilitate fluid flow. These manipulations increase handling, thereby increasing both the risk of contamination and the amount of time required to establish the fluid connection.

Metal needles employed as part of connector devices increase the risk of puncture wounds to the user. The needles used in these devices often have through-holes placed at the tip of the needle. Connection of the valve with a flow line involves piercing the needle through a sealed septum.

2

Through-holes placed at the needle tip can core the septum and release free particulates into the flow line. Such an event can prove fatal to a patient. Such through-holes may also become clogged easily with material from the septum.

Reusable connectors and adaptors are preferred for medical applications since components must often be added or removed from a fluid line connected to a patient. Reusable connectors, however, are difficult to keep sterile. Sometimes caps are employed to cover the connector to keep it sterile. Frequently, these caps are lost, or simply not used because they are not readily available when needed.

A closed, patient access system that is easy to use and employs only a valve device in communication with the patient that need not be capped or interconnected with the medical implement through a needle or adaptor, is swappable, is sufficiently durable to maintain its function after several manipulations, and maintains a fluid-tight seal at high pressures, would be of great benefit to the medical community.

SUMMARY OF THE INVENTION

The valve of this invention has several features, no single one of which is solely responsible for its desirable attributes. Without limiting the scope of this invention as expressed by the claims which follow, its more prominent features will now be discussed briefly. After considering this discussion, and particularly after reading the section entitled, "DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS," one will understand how the features of this invention provide its advantages, which include safety, reliable and repeatable performance, elimination of dead space, simplicity of manufacture and use, and employment of a valve that is swappable after use to provide sterility and has a fluid-tight seal at high pressure.

This invention is a closed, patient access system which automatically reseals after administering medication using a medical implement that directly connects with the system without the need of any intermediate needles, caps or adaptors. A two-way valve is employed utilizing a reusable seal that may be repeatedly pierced by an enclosed, protected, non-metallic spike rather than an exposed metal needle. The valve facilitates fluid, particularly liquid, transfer while maintaining sterility. The valve is easy to use and is capable of locking in place. After use, the valve is swabbed in the conventional manner with a suitable substance to maintain sterility. The design of the valve avoids accidental needle sticks. As will be discussed in detail below, the valve is useful as a medical connector or adaptor to enable liquid flow from a sealed container.

The first feature of this invention is that the valve has a body including wall structure defining an internal cavity having a proximal end and a distal end. The cavity has an open space into which the seal is pushed, and preferably has a plurality of radial indentations in the wall structure that are adjacent the seal to accommodate the expansion of the seal upon compression. The proximal end has an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through the delivery end. In most applications, the delivery end of the implement is tapered, and the wall structure adjacent the opening is tapered inward so that the wall structure and the tapered delivery end fit snug against each other upon insertion of the delivery end into the opening. The proximal end of the cavity preferably is adapted to fit snug with an ANSI (American National Standards Institute, Washington, D.C.) standard end of the medical implement. Typically, the implement is a syringe, a

5,873,862

3

connector or inlet/outlet of an IV set, or any one of a wide variety of conduits used in medical applications.

The second feature is that the spike has a tip with at least one hole located at or near the tip, and a passageway in communication with the hole that allows fluid to flow through this hole. The spike is seated inside the cavity such that the tip is inward of the proximal end and is enclosed within the cavity. Preferably, the hole is in a side of the spike adjacent the tip and is elongated, having a size of 18 gauge or greater. The tip may be sharp or slightly rounded. More than one hole is desirable for many applications, and three, symmetrically located holes inward of the proximal end are preferred. The spike may include at least one rib which allows air to enter a space between the seal and the spike, thereby facilitating the sealing of the opening when the implement is removed. The spike may have a substantially conical shape, and the seal has a complementarily, substantially conical shaped cavity within it conforming to the shape of the spike. The spike is disposed within this conical cavity and the seal covers the tip. The tip may be imbedded in the proximal end of the seal or withdrawn into the conical cavity. Preferably, the tip of the spike has a plurality of facets which meet within a recess. The preferred spike should be able to penetrate the seal repeatedly without tearing the seal. Rough edges at the tip may present a tear problem. During injection molding of the preferred plastic spike, facets of the tip will abut along a "parting line," and could form a rough edge which may tear the seal. This problem is avoided where the parting line is buried in a recess. Any rough edge at this parting line is disposed within a recess, so the seal material moves over the recess and does not contact the rough edge.

The third feature is that the resilient seal is adapted to be moved into a compressed state upon insertion of the tip of the medical implement into the opening and returns to a decompressed state upon removal of the tip. The seal in the decompressed state has a section which fills essentially completely a portion of the cavity adjacent the opening. The seal section bears against the wall structure near the opening to seal the opening. In the compressed state, the seal section is pushed by the delivery end of the medical implement away from the opening and into the cavity. A fluid tight seal is maintained between the seal section and the wall structure as the seal is moved into the compressed state. The seal section bears against the wall structure as the seal is moved inward into the cavity by the tip of the medical implement. And most importantly, the delivery end and the seal are adapted to engage so that when the tip of the spike pierces the seal there is essentially no dead space between said delivery end and the seal. Consequently, a predetermined dosage amount of medication is transferred in its entirety to the patient using this invention, with none to the prescribed amount being collected in dead space in the valve. The delivery of an exact amount of medication may be critical in some situations when chemotherapeutic agents are being administered or small children are being treated.

A fluid tight seal is maintained over repeated opening and closing of the valve, and the seal has on its external surface a recess which provides an air pocket to facilitate the movement of the seal. Preferably, the seal presents an essentially flush surface with the proximal end of the cavity. In one embodiment, the proximal end of the seal is substantially flat, the seal is made of a material having a hardness of from 30 to 70 Shore units such as, for example, a silicone polymer. The seal may include a cup-like flange adapted to engage the body near the proximal end of the cavity. A preferred embodiment of the seal comprises a series of O-ring elements stacked together and connected to form a

4

unitary structure. The O-ring elements have increasing diameters, with the smallest diameter element being adjacent the proximal end of the cavity. The proximal end of the seal may be precut to form a tiny orifice therein that allows the tip of the spike to pass therethrough easily upon compression of the seal. Preferably, the proximal end of the seal has a truncated conical shaped segment disposed within the cavity. The seal may also have a centrally located, anti-vacuum, saucer like depression therein, which does not interfere with the ability of the exposed, proximal end of the seal being swabbed when desired.

The fourth feature is that the body and spike are two separate components of the valve that are securely attached to each other by assembly of, and interlocking, of the body and spike. The body has a first locking element near the distal end of the cavity, and the spike has a second locking element adapted to interlock with said first locking element upon assembly. The seal has a lip extending beyond the distal end and positioned between the first and second locking elements so that, upon assembly, the lip is compressed between the locking elements to provide an essentially fluid tight seal upon interlocking.

The fifth feature is that the medical valve includes a support member connected to the spike which seals off the distal end of the cavity. The support member may have a Luer-Lock type connector element that enables the valve to be removably attached to, for example, a fluid line connected to a patient. The support member may also be in the form of an adaptor that enables the valve to be removably attached to a fluid dispenser or container. When used to dispense fluids from a container, the spike has a pair of opposed tips, respectively at the distal and proximal ends of the spike. The tip at the distal end of the spike pierces a cover member which seals the container. A radial slit on the adaptor enables it to deform reversibly sufficiently to fit snugly onto said container.

The sixth feature is that the seal has a proximal end including a pressure responsive element disposed on an inner surface of the seal adjacent the opening. The pressure responsive element in the decompressed state closes any orifice in the seal at the proximal end of the seal to provide an essentially fluid-tight seal while in the decompressed state. The pressure responsive element enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve is connected to a patient's artery. The valve of this invention will remain closed even when the pressure inside the valve is above 6 pounds per square inch (psi), and it can withstand pressures above 30 psi. Typically, the pressure responsive element is a section of the seal having an entryway into a precut orifice. This section has a substantially cylindrical configuration and is surrounded by an annular space which is filled with pressurized fluid. The center of the member and the annular space are coaxial with the entryway to the orifice. The pressurized fluid fills the annular space to apply pressure that compresses the cylindrical section to tightly close the entryway to the orifice. Preferably, the pressure responsive element has an anti-tear element.

In accordance with this invention, a known, prescribed, predetermined amount or dosage of medication may be transferred from the remote source to the patient directly, so that essentially none of said predetermined amount is collected in dead space in the valve. In other words essentially all the prescribed dosage is received by the patient and not lost in the valve. Thus, this invention also includes a method of transferring fluid from a remote source to a patient. This

5,873,862

5

invention also includes transfer of fluid from the patient to a remote source. This is possible because the valve of this invention provides two-way communication. The fluid is transferred to the patient by applying pressure the fluid as it passes through the implement so that the pressure applied to the fluid is greater than the pressure of fluid in the patient, enabling transfer from the remote source to the patient. To achieve transfer of fluid from the patient to the remote source, the pressure of fluid in the patient is greater than the pressure at the remote source, causing fluid to flow from the patient to the remote source. This invention also includes a method of transferring fluid in a container having an open mouth covered by a cover member which seals the open mouth. The fluid is caused to flow from the container through the passageway by creating a differential in pressure. Preferably, the valve has an adaptor having a radial slit for allowing the adaptor to deform reversibly sufficiently to fit snugly onto said container.

BRIEF DESCRIPTION OF THE DRAWING

The preferred embodiments of this invention, illustrating all its features, will now be discussed in detail. These embodiments depict the novel and non-obvious method and valve of this invention shown in the accompanying drawing, which is for illustrative purposes only. This drawing includes the following Figures, with like numerals indicating like parts:

FIG. 1 is a perspective view of the first embodiment of the valve of this invention.

FIG. 2 is an exploded perspective view of the valve shown in FIG. 1 illustrating the spike, seal, and the body or housing components of the invention.

FIG. 3 is a longitudinal cross-sectional view of the assembled valve of FIG. 1.

FIG. 4 is a schematic, longitudinal, cross-sectional view of the assembled valve of FIG. 1 before compressing the seal.

FIG. 5 is a schematic, longitudinal, cross-sectional view similar to FIG. 4 showing the valve during compression of the seal.

FIG. 6 is a perspective view of a second embodiment of the invention.

FIG. 7 is a longitudinal cross-sectional view of the valve of FIG. 6.

FIG. 8 is a schematic illustration of an ANSI delivery end of a medical implement compressing the seal of the valve of this invention.

FIG. 9 is a side elevation view, partially in cross-section, of a third embodiment of the seal.

FIG. 10 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using the seal of FIG. 9.

FIG. 11 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fourth embodiment of the seal.

FIG. 12 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fifth embodiment of the seal.

FIG. 13 is a longitudinal cross-sectional view of a sixth embodiment of the seal.

FIG. 14 is a longitudinal section of the seal shown in FIG. 13 used in connection with the spike device shown in FIG. 2.

FIG. 15 is a longitudinal partial cross-sectional view of a seventh embodiment of the seal of this invention.

6

FIG. 16 is a longitudinal cross-sectional view, after assembly, of the embodiment of the valve shown utilizing the seal of FIG. 15.

FIG. 17 is a longitudinal cross-sectional view, after assembly, of the eighth embodiment of the valve of this invention.

FIG. 18 is a longitudinal cross-sectional view, after assembly, of the ninth embodiment of the valve of this invention.

FIG. 19 is a side elevation view, after assembly, of the seal and spike shown in FIG. 14 connected to the body or housing shown in FIGS. 20 and 21.

FIG. 20 is a cross-sectional view taken along line 20—20 of FIG. 19.

FIG. 21 is a perspective view, with sections broken away to show the wall structure of the cavity containing the seal shown in FIGS. 13 and 14.

FIG. 22 is a greatly enlarged, cross-sectional view taken along line 22—22 of FIG. 14.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

The term “proximal” is used to denote the end of the valve and other components at or near the spike tip 32 in FIGS. 2 through 5, 10 through 12, 14, and 16, and at or near the spike tip 60 in FIG. 6, and at or near the seal cap 92 in FIGS. 8, 9, 13 through 19. The term “distal” is used to denote the opposite end of the valve, or spike tip, or seal. The term “medical implement” is used to denote any medical tool known to those of skill in the art that can connect to the present invention and facilitate the passage of fluids, particularly liquids, through the instant invention. Examples of medical implements that are contemplated include, but are not limited to, tubing, conduit, syringes, IV sets (both peripheral and central lines), piggyback lines, and other components which can be used in connection with a medical valve. Medical implements are commercially available in standard sizes. Thus, either or both ends of the valve of this invention can be provided with fittings to accommodate such standard size medical implements.

As best shown in FIGS. 1 and 2, the first embodiment of the invention, valve 10, includes a valve body or housing 12, a spike element 24, and a seal 36. The seal 36 is prepared from a resilient material that is flexible, inert, impermeable to fluid, and readily pierceable by the spike 26. In the embodiment shown in FIG. 13 depicting an alternate shaped seal 36d, this seal 36d has a precut slit 11 in its proximal end. This provides a tiny orifice through which the tip 32 of the spike element 24 may easily pass, yet still provides a fluid tight seal upon withdrawal of the spike element. These three components are assembled, as depicted in FIG. 3, with the spike element 24 enclosed to prevent accidental sticks. FIG. 2 illustrates how the housing 12, seal 36, and spike element 24 are attached without the need to use any adhesive or other bonding agent or process. Mechanical connection which provides a fluid tight closure is attained as is discussed subsequently. As shown in FIGS. 4 and 5, the seal 36 moves within the housing 12, being pierced by the spike element 24 to expose the tip 32 of the spike element 24 to allow fluid to flow through the valve 10.

Referring to FIG. 1, one preferred embodiment of housing 12 has a bell-shaped skirt 16 and an upper, preferably cylindrical, conduit 20. The skirt 16 is integral with, and connected by an annular ring 14, to the upper conduit 20. The skirt 16 creates a shield for an inner conduit 18 of the

5,873,862

7

spike element 24. This inner conduit 18 is preferably cylindrical in shape, and slightly tapered. Inner conduit 18 and upper conduit 20 comprise aligned hollow tubes so that inner conduit 18 and upper conduit 20 are in fluid communication with one another when the spike element 24 pierces the seal 36. There is an annular lip 25 surrounding a circular opening 25a in the top of the conduit 20 (see FIG. 2).

In the first embodiment, the upper conduit 20 is adapted to receive the tip or nose 48 of an ANSI standard syringe 46 (see FIGS. 4 and 5). It is, however, contemplated that the outer diameter of the upper conduit 20 can be of any size to accommodate the attachment of other connector devices thereto. Advantageously, the proximal end of the upper conduit 20 can be equipped with a locking mechanism to facilitate locking of the valve 10 to a variety of connector devices. For example, referring to FIG. 1, locking ears 22 near the proximal lip 25 of housing 12 are preferably provided such that the housing 12 can be locked into any compatible Luer-Lock device known to those with skill in the art. For example, referring to FIG. 19, conventional Luer-Lock threads 180 can be provided on the outer diameter of upper conduit 20.

Referring to FIG. 2, the spike element 24 has at its distal end the inner conduit 18 and at its proximal end a hollow spike 26 which is integral with the inner conduit. The inner conduit 18 and spike 26 present a continuous passageway for fluid during use. An annular cuff 28 on an intermediate portion of the spike element 24 is integral with, and interconnects, the inner conduit 18 and the spike 26. As illustrated in FIG. 3, the rim 28a of the cuff 28 abuts the underside of the inner ring 14, and has an annular detent 28b that snaps into an annular groove 14b in the underside of the ring. The cuff 28 serves two functions. First, it serves as an attachment device to the underside of the annular ring 14. Second, it serves as a support and attachment device for the seal 36.

The hollow spike 26 has a tapered conical shape, ending in a sharp, pointed tip 32. Preferably, along the length of the spike are raised, protruding ridges 30. These raised ridges 30 extend from the surface of the spike preferably between 0.2–2.0 mm. The ridges 30 are preferably aligned along the length of the spike as illustrated in FIG. 2. These ridges 30 serve to break any vacuum created when the spike 26 is sealed as described hereinbelow. Modifications to the alignment and orientation of the ridges are discussed hereinbelow in association with their function. Just distal the spike tip 32, there is situated at least one longitudinal through-hole 34 to permit fluid communication between the inner conduit 18 and the upper conduit 20. Preferably, there are three through-holes 34 within about 0.200 inch from the spike tip 32. These through-holes 34 may be of any size, however, the larger the size of the through-holes the greater the fluid flow rate through the valve 10. In a preferred embodiment, the size of the through-holes 34 are 18-gauge to provide a flow rate three times that of a standard 18 gauge needle.

The seal 36 has a seal cap 40 with a generally flat top surface 40b, an outwardly tapered sidewall 38, and a lower lip 42. Its interior is hollow to provide the conically shaped cavity 37 (FIG. 3). Thus, the seal 36 slips easily over the spike element 24 to fit snugly within the cavity 37. The seal lip 42 is seated within the annular cuff 28 and wedged between the cuff and the underside of the ring 14. There are longitudinal grooves 43 (FIG. 2) along the length of the seal 36 which provide air pockets that facilitate compression of the seal 36 during use. The grooves 43 may be of variable shape or size to facilitate seal compression. In the first embodiment, there is a single groove 43 which completely surrounds the seal 36 between the seal cap 40 and the lip 42.

8

The base of the seal 36 has a width such that the seal lip 42 fits snugly into the annular cuff 28. The hollow interior or cavity 37 (FIG. 3) of the seal 36 is preferably tapered to conform internally to the shape of the spike 24, having a wall portion 44 which contacts the spike 24 distal seal cap 40. The exterior of the seal 36 is sized and shaped to fit inside the upper conduit 20 of the housing 12. The cap 40 reseals the valve 10 when the top surface 40b is above the through-holes 34. Preferably, the cap 40 substantially fills the opening 25a in the top of the conduit 20. Thus, after assembly, the top surface 40b of the seal cap 40 is essentially flush with the lip 25, so that the lip 25 and seal cap 40 can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve 10. It is important that the surface 40b be exposed so that it may be swabbed with a disinfectant.

As best shown in FIG. 3, the spike 24, with contiguous inner conduit 18, is affixed to the housing 12 through the association of the external portion of annular cuff 28 and the internal portion of annular ring 14. Although not necessarily required, these two pieces may be affixed by any one of a variety of methods known to those of skill in the art including, but not limited to, heat sealing, glue, pressure lock, bonding or the like. The seal 36 fits into the annular cuff 28 and is held in place by an internal lip 27 along the internal portion of the annular ring 14 of the housing 12. The length of the spike 24 is such that, after assembly, the tip of the spike rests below the plane defined by the lip 25 of the housing 12. Preferably, the spike tip 32 is approximately from 0.525" to 0.1" below the lip 25 of the housing 12. The seal 36 fits snugly against the spike 24 and is essentially flush with the lip 25 of the housing 12. The spike tip 32 is thus embedded within the seal cap 40 prior to use or may be approximately 0.025" distal the seal cap 40 when the valve 10 is in the closed position. The inner conduit 18 is partially shielded by the bell shaped skirt 16 of the housing 12 (see FIGS. 1–3). The inner surface of the bell shaped skirt 16 preferably has protruding threads 44 as an optional locking mechanism for attaching a medical implement thereto. Further, other medical devices can be pressure fit over the outer portion of inner conduit 18 without direct association with the protruding threads 44.

During use, the invention is designed to be adapted as a two-way valve. The orientation of the valve is independent to fluid flow and dependent on the preferred orientation of the preexisting connections. Thus, the invention can be used as a valve connector for an intravenous central or peripheral piggyback connector in either orientation. Parenteral fluid is delivered to patients through tubing such that the liquid flows from a container through a needle into the patient. The containers are frequently changed or additional fluid bottles are added. The invention disclosed herein is designed to interconnect medical implements along the route of fluid delivery to the patient. However, the invention is also useful in any environment in which a resealable fluid valve is desired. During use, a connector of the appropriate size is fitted over the inner conduit 18. Locking can be achieved by a Luer-Lock mechanism, a pressure fit or any other locking mechanisms known to those with skill in the art, as described above. Thus, in one example, fluid passes from the inner conduit 18 into the spike 26. However, fluid flow is locked in place by the seal 36.

FIGS. 4 and 5 illustrate valve activation. In FIG. 4, the medical implement connecting to the proximal end of the valve 10 is a syringe 46. However, this connecting implement could be any number of medical implements known to those of skill in the art. The nose 48 of the syringe 46 is placed on the seal cap 40 inside the lip 25 of the housing 12.

5,873,862

9

The application of pressure on the syringe **46** in the direction of the arrows, as illustrated in FIG. **4** creates pressure on seal cap **40**. The resulting downward pressure compresses the seal **36**. This pushes the tip **32** of the spike **26** through the seal cap **40** to expose the through-holes **34**. Compression is facilitated by the grooves **38**. Fluid is now able to flow into the syringe **46**, or vice versa, depending on whether fluid is to be withdrawn from the patient or medication injected into the patient. FIG. **5** shows valve **10** opened by insertion of the nose **48** of the syringe **46** into the opening **25a**. A syringe plunger **49** in the syringe **46** is retracted thereby creating a vacuum to draw fluid through the valve **10** into the syringe. For intravenous applications, the valve **10** can be orientated in the position diagramed in FIGS. **4** and **5**, or it can be rotated 180° such that fluid flows in the opposite direction.

Upon removal of the syringe from spike **26**, as shown in FIG. **4**, the seal **36** is free to return to its original shape and cover through-holes **34**. The ability of the seal **36** to return to its original shape is determined by the resiliency of the material used to prepare the seal **36**. In addition, the ability of the seal **36** to return to its original shape is facilitated by the protruding ridges **30** formed on the external surface of the spike. During compression, a vacuum may form in the area between the spike **26** and the seal **36**, thereby preventing the seal **36** from returning to its original position. The protruding ridges permit air to pass along the spike/seal interface to prevent vacuum formation and allow free return of the seal. The ability of the seal **36** to deform reversibly and return to its original position is particularly useful because (1) it immediately stops fluid flow through the valve **10**, (2) it covers the recessed spike **26** to maintain its sterility, and (3) it reduces the risk that the spike could inadvertently pierce another object or person. In addition, since the valve **10** lacks movable parts, except for the seal, it is unlikely that when the seal **36** is pushed down, the valve **10** would fail to function.

Advantageously, the through-holes **34** are located relatively low on the spike **26**. Thus, the through-holes **34** are sealed relatively early in the process as the seal **36** returns to its original configuration with the valve **10** is closed. In one preferred embodiment the through-holes **34** are located 0.075" below the spike tip **32** (see FIG. **2**). Additionally, the through-holes **34** are sealed even if the seal **36** does not fully return to its original configuration depicted in FIG. **4**. Further, the ability of the seal **36** to return reversibly to its original position permits the reuse of the connector valve **10**. Following disconnection, and before reuse, the surface of pierced seal cap **40** is essentially flush with the housing **12**. Thus, this flush surface can, advantageously be sterilized with alcohol or other surface decontaminating substances. The skirt **16** and upper conduit **20** advantageously shield both connections from the surrounding environment to protect the sterility of the connection. Further, both the skirt **16** and upper conduit **20** function as collection reservoirs to prevent fluid from dripping from the valve **10** during manipulation.

A cover cap (not shown) can be supplied to fit over the upper conduit **20** as further protection for the seal surface between use. Such a cover cap, however, is not needed to maintain sterility since the seal **36** may be swabbed with a disinfectant after each use. The reversibility of the seal **36** makes the valve **10** particularly attractive as a connector valve to provide fluid communication between two fluid lines. Therefore, the present invention provides for placing a first fluid line in communication with a second fluid line using the valve disclosed herein. The reversibility of the valve **10** permits multiple fluid lines to be successively

10

added, for example, to a fluid line in direct communication with a patient's vein. Since the valve is easily sterilizable and sealable, fluid lines can be added and removed without disconnecting venous contact.

The valve **10** is preferably prepared from a hard plastic, but it is additionally contemplated that the valve could be prepared from other medically inert materials known to those in the art. The spike element **24** is preferably prepared from the same material as the housing **12**. One particular advantage of this invention is that it does not rely on the use of metal needles. This dramatically reduces the risk of skin puncture during use and manufacture. Further, the upper conduit **20** serves as a shield to the spike **26** such that skin puncture is further reduced. The spike **26** need only be strong enough to penetrate the seal cap **40**, or if necessary, to pierce a connecting septum.

In the embodiment of the invention illustrated in FIGS. **2-4**, the through-holes **34** are placed distal spike tip **32**. This placement provides two important advantages. First, the placement of the through-holes **34** facilitates resealing of the valve **10** after use. Second, if the through-holes were placed at the spike tip **32**, the holes **34** may core the seal cap **40** thereby introducing seal particulate into the fluid flow and possibly plugging the holes **34**. Thus, the longitudinal placement of the through-holes distal spike tip **32** prevents the introduction of particulates into the fluid path and/or plugging of the through-holes **34**. It is additionally contemplated that the number and diameter of the through-holes **34** can be adjusted to accommodate different fluid velocities. In a preferred embodiment, the preferred velocity of fluid passing through the through-holes **34** is equal to or greater than the flow rate through an **18** gauge needle. Through-holes larger than **18** gauge will, of course, facilitate greater fluid velocities.

An important advantage of the invention is that the valve **10** has very little dead space, thus the volume of liquid entering into the valve is substantially equivalent to the volume of fluid leaving the valve. Further, the total equivalent fluid volume of the valve is very small such that the volume of fluid flowing through the system in order to place the valve in fluid communication with a medical implement such as a syringe **46** is substantially zero.

ALTERNATE EMBODIMENTS

In another preferred embodiment of the invention, illustrated by FIGS. **6** and **7**, a disposable sterile adaptor valve **50** is provided to function as a resealable lid for a container (not shown) of fluid. The fluid can thus be removed from the fluid container or permitted to flow from the container into a medical implement adapted to house fluid in a sterile manner. As is the conventional practice, an open mouth of the container will ordinarily be sealed with a cover member (not shown).

FIG. **6** shows an adaptor valve **50** having a body including an adaptor skirt **52**. The adaptor skirt **52** will preferably fit snugly over the open mouth of the container. The skirt **52** may be of any size to accommodate a range of container sizes. A lengthwise slit **54** is preferably provided in at least one location along the length of the skirt to ensure a snug fit between the skirt **52** and the container. A chamber **56**, preferably tubular in configuration, extends upward from the skirt **52** and is similar in construction and design to the upper chamber **20** of the first preferred embodiment. Similar to the first embodiment, the proximal portion of the valve contains a locking mechanism **59** that preferably comprises a Luer-Lock device or other locking device known to those of skill in the art.

5,873,862

11

As depicted in FIG. 7 a spike 58 extends upward through a tubular chamber 56. A spike tip 60 is preferably recessed from a proximal lip 62 of the tubular chamber 56. In a closed position, this tip 60 is covered by a seal 64, which is essentially the same as seal 36. Protruding ridges 66 and seal grooves 68 facilitate seal compression in the open position and promote closure following use. Thus, in the closed position as illustrated in FIG. 7, the seal 64 covers the through-holes 70 to prevent fluid out-flow from the container. The adaptor valve 50 contains a second spike 72 which points in the opposite direction as spike 58. These spikes 52 and 72 are in fluid communication with each other. The spike 72 extends downward inside the adapter skirt 52. The two spikes preferably form one component of the valve 50 while the skirt 52 and upper chamber form a second component. These two components can be assembled in a manner like that of the valve 10. The spike 72, like the spike 58, has longitudinal through-holes 74 and a tip 76. The through-holes 74 are located inward of the tip 76. The adaptor valve 50 is thus useable with containers holding sterile medicament having a cover or septum seal at the open mouth of the container. Examples of containers with such seals contemplated for use with this invention include dosage bottles for intramuscular injector antibiotic containers or the like. However, it is also contemplated that the valve 50 can be adapted with its own seal and locking mechanism to permit the valve to be employed on a variety of containers for medicaments or other fluids. Medicaments in these types of containers are preferably maintained under sterile conditions and the volume and nature of the medicament is such that multiple aliquots are intermittently removed over time. If the medicament is reconstituted, then, during use, any covering over the opening on the container is removed to reveal the rubber septum. The adaptor valve 50 is placed over the septum and direct pressure is applied to pierce distal spike 72 through the septum and into the container. A syringe or the like can then be applied, as depicted in FIG. 4, in association with the first preferred embodiment, to withdraw fluid from the container. The pressure of the nose 48 over the spike 58 pushes spike tip 60 through seal 64. At the same time, seal 64 is pushed back and compresses. Compression is accommodated by seal grooves 68. Fluid is withdrawn from the container and the syringe is removed from the spike 58. Release of the pressure applied to seal 64 permits the seal to return to its original configuration. The spike ridges 66 facilitate seal reversibility.

Often the ingredients housed in containers are those that can be lyophilized at purchase. Lyophilized ingredients require reconstitution before use. If the medicament requires reconstitution before use, then sterile water, saline, or other fluid can be introduced into the container before fluid is extracted. The two-way nature of the valve permits this without any special adaptation. After the syringe is removed, the adaptor valve 50 automatically seals. Subsequently, aliquots can be removed from the container by syringe or the like. Alcohol or other compatible surface sterilizing agent can be used to wipe the lip 62 and seal 64 before each use. Similar to the first embodiment, it is additionally contemplated that a cap can be provided to fit over upper chamber lip 62 between use.

The adaptor valve 50 can be adapted to function as a medicament adaptor for an intravenous container. In this case, the adaptor valve 50 is placed on a medicament container for intravenous delivery and attached via tubing to an intravenous feed. Thus, the adaptor valve 50 can be placed in fluid communication with a connector valve of FIG. 1 to facilitate the flow of medicament from intravenous drip bottles.

12

An alternative embodiment of the seal, a seal 36a, is shown in FIG. 9. Seal 36a comprises a seal cap 92 at the proximal end thereof and a seal lip 96 at the distal end thereof. A cup-like annular flange 95 is provided proximal seal cap 92. The seal cap 92 and seal lip 96 are connected by a seal wall consisting of a plurality of ringed wall portions 94 that expand and collapse in an accordion like fashion. During compression of the seal 36a, the diameter of the ringed wall portions 94 expand outward in the radial direction. There are air pockets 13a (FIG. 10) between ring portions 94 and the housing and air pockets 13b between spike 24 and seal 36a. The seal 36a contains a cavity 98 distal seal cap 92 and adjacent the ringed wall portions 94. The seal 36a interacts with spike 26 (FIG. 2) and other components of the present invention in a similar fashion to seal 36 of FIG. 2.

Referring to FIG. 10, the cup-like annular flange 95 may be stretched around the upper conduit 20 and held in place by an annular ring 97. This creates a trampoline like effect that assists returning the seal 36a to a decompressed state after withdrawal of a syringe (not shown). This embodiment has two advantages. First, the proximal end of the valve 10 can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve 10. Second, by affixing cup-like annular flange 95 to upper conduit 20 at the proximal end thereof with annular ring 97, the repeated deformation and reformation of the seal 36a is assisted.

An alternative embodiment of the seal, a seal 36b is shown in connection with the valve 10 in FIG. 11. S The seal 36b is similar to the seal 36a and is comprised of seal cap 92, a side wall consisting of ringed wall portions 94 and a seal lip 96. It also has an outwardly extending ring 99 which is at a right angle with respect to the longitudinal axis of the valve 10. This ring 99 is used to attach the seal 36b to upper conduit 20. Preferably, an upper conduit annular plug 20' is inserted within upper conduit 20 to create a tight fit between perpendicular ring 99, a ledge 101 in the upper conduit 20, and the plug 20'. The ring 99 assists in the reformation of seal 36b to enclose spike 26 upon withdrawal of a syringe (not shown).

As shown in FIG. 12, the cup-like annular flange 95 and ring 99 may both be used in connection with the valve 10, to provide the seal 36c. This seal 36c, provides rapid reformation upon withdrawal of a syringe (not shown) and realizes the advantages of both the seals 36a and 36b.

Another alternative embodiment of the seal, a seal 36d, is shown in FIG. 13. In this embodiment, the seal 36d is comprised of seal cap 92, seal lip 96, and a side wall 150 comprised of circular tires 100 stacked in series one on top of an adjacent larger diameter lower tire. The circular tires 100 are preferably solid throughout the diameter of the cross-section thereof. These circular tires 100 will deform and reform upon, respectively, compression and decompression of the seal 36d, thereby exposing or covering a spike (not shown) as the case may be.

As mentioned above, preferably seal 36d has a precut slit 11 in the cap 92 lying along the longitudinal axis of the valve 10. The seal cap 92 has a unique configuration that insures that the slit 11 closes and is sealed upon withdrawal of a syringe (not shown) and reformation of the seal 36d. It includes an enlarged, internal, pressure responsive member 200 which is integral with the cap 92. Between the proximal end of the side wall 150 and the member 200 is an annular space 102 which is filled with the fluid in the cavity 98. This fluid is under pressure, for example at the blood pressure of the patient to which the valve 10 is attached. Referring to

5,873,862

13

FIG. 14, fluid, for example the patient's blood, flows through the holes 34 in the spike 26, filling the cavity 102. This fluid presses against the exterior of the member 200, closing the slit 11 when the seal is decompressed as shown in FIGS. 14 and 19. The pressure from this fluid creates a high pressure seal which prevents fluid from escaping valve 10 through the slit 11. There is a semi-cylindrical annular flange tear ring 104 on the end of the member 200 which advantageously extends the useful life of seal 36d.

Preferably, there is a tear ring 104 integral with the member 200 along the perimeter of the internal surface the member 200, and a slight saucer-like depression 204 in the external surface of the seal. The pressure responsive element in the decompressed state closes any orifice in the seal 36d to provide an essentially fluid-tight seal while in the decompressed state. The pressure responsive member 200 enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve 10 is connected to a patient's artery. The center of the member 200 and the annular space 102 are coaxial with the entryway 11a to the orifice 11. The pressurized fluid fills the annular space 102 to apply pressure that compresses the member 200 to tightly close the entryway to the orifice. In a preferred embodiment the distance from the entryway 11a to the proximal end of seal cap 92 is from 0.500 to 0.075 inches and more preferably approximately 0.100 inch.

As best illustrated in FIG. 22, the tip 32 is designed to avoid tearing the seal. Tip 32 has three facets 210, 212, and 214 which are joined with each other along parting lines a, b, and c. This junction of the facets 210, 212, and 214 frequently is ragged and will tear the seal 36d. This is prevented by the parting lines a, b, and c, or junctions, being disposed within recesses 220, 222, and 224, respectively, to provide "buried parting lines."

Another alternative embodiment of the present invention using the seal 36d is shown in FIG. 8 and FIGS. 19 through 21. In this embodiment, the inner wall 160 of the upper end of the conduit 20 is provided with at least one, and preferably, a plurality of radial indentations 107. The indentations 107 are elongated disposed generally parallel to the longitudinal axis of the valve 10 in a symmetrical, star-like configuration. Each indentation has opposed lateral edges 162 which engage the seal 36d upon compression of the seal 36d. The indentations provide space into which the seal 36d expands upon compression.

As best shown in FIG. 8, the wall 181 of the proximal end of the conduit 20 is tapered inward at the same angle as the nose 48 of the syringe 46. In accordance with ANSI standards, the taper is 0.006 inch per linear inch. The wall 182 of the syringe nose 48 bears against the wall 181 as the nose slides into the opening 25a to push the seal 36d inward compressing it and forcing the tip 32 of the spike 36 to enter the slit 11. The seal 36d expands upon compression to fill essentially completely the upper portions of the indentations 107. Some sections of the seal 36d are wedged between the edges 162 and other sections fill the indentations 107. As the liquid flows through the nose 48 through holes 34, air in the nose 48 is forced out of the nose 48 and expelled from valve 10 between walls 181 and 182. Thus, essentially the entire prescribed dosage is delivered through valve 10 to the patient. Fluid flows through the through-holes 34, but does not leak between either the seal 36d and the wall 181 or between the abutting walls 181 and 182.

FIGS. 15, 16, 17, and 18 depict embodiments of seals, namely, seal 36e, seal 36f, and seal 36g, which are substantially the same as the seals 36a (FIG. 10), seal 36b (FIG. 11), and seal 36c (FIG. 12), except the side wall 150 employing the circular tires 100 is used in place of the accordion wall portion 94.

14

Other components of the present invention interact with the various embodiments of the seal in a similar fashion to their interaction with seal 36 of FIG. 2. Prior to use of valve 10, it is preferable that the seal caps 40 or 92 be pierced centrally by a steel needle in the axial direction, precutting the seal to provide the slit 11 in order to allow for more rapid decompression and reformation of the seal upon piercing by the spike 26. The seals are advantageously formed from a material which can repeatedly reseal and prevent fluid from flowing around the seal material. The seal 36 should also be capable of being forced down and then spring back into position to reseal the valve. Material that is too soft will reseal effectively; however, will not be capable of springing back after opening of the valve. Material that is too hard will provide sufficient spring force; however, will not effectively seal. Thus, in a preferred embodiment, the seal is formed from a silicone having a hardness in the range from 30–70 Shore durometer units, and more preferably in the range 40–50 Shore durometer units. A cure silicone polymer in the preferred hardness range is available from Wacker Silicone Corp. of Adrian, Mich. In some embodiments of the invention, it is desirable to provide additional lubricity to the seal 36 to allow it to spring back and reseal more effectively. Dow Chemical Co. produces a silicone formulation with silicone oil built in to provide this additional lubricity.

In general, the closing of the valve 10 is provided not by the side wall of the seal 36 which immediately covers the through-holes 34, but by the seal cap 40, or seal cap 92 filling the proximal end of the cavity 98 and the opening 25a. Thus, the seal caps 40 and 92 are sufficiently thick to reseal the opening 25a effectively after valve closure. However, the seal caps 40 and 92 should also be sufficiently thin to allow them to readily return to the closed position. Preferably the thickness of the caps 40 and 92 ranges; between 0.075 and 0.500 inch and more preferably may be approximately 0.100 inch.

The valve disclosed in this invention can be provided in a sterile and disposable form such that after its use in a given installation is exhausted, the device is discarded. However, as described above, in any given installation, the device can be reused multiple times. Since the device does not employ needles, there is little chance that the device will inadvertently cause skin puncture. Therefore, the extra precautions required for handling and disposing of needles is obviated. It will be apparent from the detailed description provided herein that the present invention can provide for the elimination of nearly all needles used in the medical environment. With the use of the valve of the present invention, the need for all needles except those that are directly input into a patient is, advantageously, eliminated.

OPERATION

The valve 10 is used to provide a closed, patient access system for transferring a predetermined amount of medication from a remote source to the patient. The valve 10 is connected by the distal end to the patient, for example, a vein or artery in fluid communication with the valve. Blood fills the valve, but the seal 36d, for example, prevents any blood from leaking from the valve. The delivery end or nose 48 of the medical implement is inserted into the valve as depicted in FIG. 8, pushing the nose 48 against the seal to compress the seal sufficiently to allow the tip 32 of the spike 24 to pierce the seal and enter said delivery end. The predetermined amount of medication in its entirety may now be transferred through the nose 48 into the valve 10 and into the patient. Since the nose 48 and seal 36d engage in a manner so that the tip 32 of the spike element 24, upon piercing the seal, meets the seal to avoid formation of any dead space at the interface between nose 48 and the seal surface 40b. Transfer directly through the valve 10 of

5,873,862

15

essentially the entire predetermined amount of medication from the syringe **46** to the patient, so that essentially none of said predetermined amount is collected in any dead space in the valve, is accomplished with this invention. Upon withdrawing the nose **48** from the valve **10** the seal **36d** returns to the decompressed state to close the valve and maintain while in said decompressed state a fluid tight seal even at high pressures and after repeated uses.

SCOPE OF THE INVENTION

The above presents a description of the best mode contemplated of carrying out the present invention, and of the manner and process of making and using it, in such full, clear, concise, and exact terms as to enable any person skilled in the art to which it pertains to make and use this invention. This invention is, however, susceptible to modifications and alternate constructions from that discussed above which are fully equivalent. Consequently, it is not the intention to limit this invention to the particular embodiments disclosed. On the contrary, the intention is to cover all modifications and alternate constructions coming within the spirit and scope of the invention as generally expressed by the following claims, which particularly point out and distinctly claim the subject matter of the invention.

I claim:

1. A method of transferring fluid from a remote source to a patient, comprising:

(a) connecting a medical valve to the patient, wherein the valve comprises a body including wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end, a spike having a tip, at least one hole located at or near said tip, and a passageway in communication with the hole that allows fluid to flow through said hole, said spike being seated inside the cavity such that said tip is enclosed within the cavity, and a resilient seal having a proximal end and a distal end and adapted to be moved distally in the cavity into a compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to a decompressed state upon removal of said delivery end from said opening, said seal in the decompressed state having a section which fills essentially completely a portion of the cavity adjacent said opening, said seal section bearing against said wall structure near said opening to seal said opening, and in the compressed state said seal section being located in the cavity distal said opening, said seal being preslit at the proximal end thereof, wherein said seal has at least one horizontal groove to facilitate the movement of the seal;

(b) inserting the delivery end of the medical implement into said opening; and

(c) pushing said delivery end into the cavity to compress said seal sufficiently to allow fluid to flow from said medical implement through said valve to the patient.

2. A method of transferring fluid from a remote source to a patient, comprising:

(a) connecting a medical valve to the patient, wherein the valve comprises a body including wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end, a spike

16

having a tip, at least one hole located at or near said tip, and a passageway in communication with the hole that allows fluid to flow through said hole, said spike being seated inside the cavity such that said tip is enclosed within the cavity, and a resilient seal having a proximal end and a distal end and adapted to be moved distally in the cavity into a compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to a decompressed state upon removal of said delivery end from said opening, said seal in the decompressed state having a section which fills essentially completely a portion of the cavity adjacent said opening, said seal section bearing against said wall structure near said opening to seal said opening, and in the compressed state said seal section being located in the cavity distal said opening, said seal being preslit at the proximal end thereof, wherein said seal has at least one groove defined by at least two O-ring elements forming a portion of said seal to facilitate the movement of the seal;

(b) inserting the delivery end of the medical implement into said opening; and

(c) pushing said delivery end into the cavity to compress said seal sufficiently to allow fluid to flow from said medical implement through said valve to the patient.

3. The method of claim **2**, wherein each succeeding O-ring element in the distal direction has a larger diameter than the preceding O-ring element.

4. A method of transferring fluid from a remote source to a patient, comprising:

(a) connecting a medical valve to the patient, wherein the valve comprises a body including wall structure defining an internal cavity wherein said body has a plurality of radial indentations in an interior wall of said body and said internal cavity has a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end, a spike having a tip, at least one hole located at or near said tip, and a passageway in communication with the hole that allows fluid to flow through said hole, said spike being seated inside the cavity such that said tip is enclosed within the cavity, and a resilient seal having a proximal end and a distal end and adapted to be moved distally in the cavity into a compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to a decompressed state upon removal of said delivery end from said opening, said seal in the decompressed state having a section which fills essentially completely a portion of the cavity adjacent said opening, said seal section bearing against said wall structure near said opening to seal said opening, and in the compressed state said seal section being located in the cavity distal said opening, said seal being preslit at the proximal end thereof, wherein said seal has a groove to facilitate the movement of the seal;

(b) inserting the delivery end of the medical implement into said opening; and

(c) pushing said delivery end into the cavity to compress said seal sufficiently to allow fluid to flow from said medical implement through said valve to the patient.

5. The method of claim **4**, wherein said seal expands into said radial indentations upon distal compression of said seal.

* * * * *

Disclaimer

5,873,862—George A. Lopez, Corona del Mar, Calif. MEDICAL VALVE AND METHOD OF USE.
Patent dated Feb. 23, 1999. Disclaimer filed September 07, 2006. by the Assignee, ICU Medical, Inc.

The term of this patent shall not extend beyond the expiration date of Pat. No. 5,685,866.
(*Official Gazette May 22, 2007*)

EXHIBIT C



US005928204A

United States Patent [19]
Lopez

[11] **Patent Number:** **5,928,204**
[45] **Date of Patent:** **Jul. 27, 1999**

[54] **MEDICAL VALVE AND METHOD OF USE**

WO 93/11828 6/1993 WIPO .

[75] Inventor: **George A. Lopez**, Corona del Mar, Calif.

[73] Assignee: **ICU Medical, Inc.**, San Clemente, Calif.

[21] Appl. No.: **08/488,106**

[22] Filed: **Jun. 7, 1995**

Related U.S. Application Data

[63] Continuation of application No. 08/334,846, Nov. 4, 1994, Pat. No. 5,685,866, which is a continuation of application No. 08/096,659, Jul. 23, 1993, Pat. No. 5,695,466, which is a continuation-in-part of application No. PCT/US92/10367, Dec. 1, 1992, abandoned, which is a continuation-in-part of application No. 07/813,073, Dec. 18, 1991, abandoned.

[51] **Int. Cl.**⁶ **A61M 5/00**

[52] **U.S. Cl.** **604/249; 604/256**

[58] **Field of Search** 604/246, 249, 604/247, 256, 283, 216

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 321,250 10/1991 Jepson et al. .
D. 321,251 10/1991 Jepson et al. .
1,578,517 3/1926 Hein .
2,289,677 7/1942 Perelson .
2,847,995 8/1958 Adams .

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

1105959 7/1981 Canada .
0 114 677 A2 8/1984 European Pat. Off. .
0 237 321 3/1987 European Pat. Off. .
0 240 987 A2 10/1987 European Pat. Off. .
0 309 771 A1 9/1988 European Pat. Off. .
0 446 463 A1 12/1990 European Pat. Off. .
84 25 197 U 9/1985 Germany .
WO 86/01712 3/1986 WIPO .
WO 86/03416 6/1986 WIPO .

OTHER PUBLICATIONS

Nita I.V. Standards of Practice, pp. 71, 72 and Exhibit A, showing Nutri-Flo Product, vol. 5, Jan.-Feb. 1982.

Baxter Product Brochure, "Closed Draining Bag", 2 pages.

Baxter Product Brochure, "Urine Sampling Unit", 2 pages.

Travenol Laboratories, Inc., Product ad, "Mini-Bag Under-fill Vialflex Containers", 3 pages.

Nita, vol. 7. No. 2 Mar./Apr. 1984, 6 pages.

Travenol Ad, "The Continu-Flo Administration System", 4 pages.

American Journal of Hospital Pharmacy, vol. 26, Jan. 1969, 12 pages.

American Journal of Hospital Pharmacy, vol. 36, Nov. 1979, 7 pages.

American Society of Hospital Pharmacists "Evaluation of Piggyback Administration Sets", vol. 34, Dec. 1977, pp. 1315-1323.


Primary Examiner—Corrine M. McDermott

Attorney, Agent, or Firm—Knobbe, Martens, Olson & Bear, LLP

[57] **ABSTRACT**

A closed system, needleless valve device includes a generally tubular body defining an internal cavity. On the proximal end of the body there is an opening which is preferably sufficiently large to receive an ANSI standard tip of a medical implement. The distal end of the body has a generally tubular skirt. The valve also includes a hollow spike having a closed tip. The spike includes at least one longitudinal 18-gauge hole located distal the tip, and is seated inside the cavity such that the tip is below the proximal end of the body. An annular support cuff is connected to the spike which seals off a portion of the cavity of the body such that an upper cavity containing the tip is defined. The valve also includes a plastic, resilient silicone seal which fills the upper cavity and opening and covers the tip of the spike so as to present a flush surface. An adaptor enables the valve to be attached to a resealable container.

12 Claims, 19 Drawing Sheets

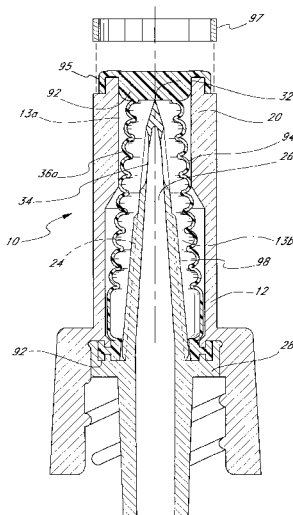

5,928,204

Page 2

U.S. PATENT DOCUMENTS


3,134,380	5/1964	Armao .	4,673,400	6/1987	Martin .
3,135,261	6/1964	Carroll .	4,706,487	11/1987	Bandou et al. .
3,354,881	11/1967	Bloch .	4,725,267	2/1988	Vaillancourt .
3,648,684	3/1972	Barnwell et al. .	4,752,292	6/1988	Lopez et al. .
3,852,385	12/1974	Huggins .	4,775,369	10/1988	Schwartz .
3,974,832	8/1976	Kruck .	4,781,702	11/1988	Herrli .
3,976,063	8/1976	Henneman et al. .	4,810,241	3/1989	Rogers .
3,986,508	10/1976	Barrington .	4,826,500	5/1989	Rautsola .
4,019,512	4/1977	Tenczar .	4,846,809	7/1989	Sims .
4,076,285	2/1978	Martinez .	4,874,377	10/1989	Newgard et al. .
4,079,738	3/1978	Dunn et al. .	4,950,260	8/1990	Bonaldo .
4,080,965	3/1978	Phillips .	4,964,855	10/1990	Todd et al. .
4,121,585	10/1978	Becker, Jr. .	4,969,883	11/1990	Gilbert et al. .
4,128,098	12/1978	Bloom et al. .	4,981,469	1/1991	Whitehouse et al. .
4,161,949	7/1979	Thanawalla .	4,998,713	3/1991	Vaillancourt .
4,187,846	2/1980	Lolachi et al. .	4,998,921	3/1991	Vickroy et al. .
4,219,912	9/1980	Adams .	4,998,927	3/1991	Vaillancourt .
4,328,802	5/1982	Curley et al. .	5,069,225	12/1991	Okamura .
4,334,551	6/1982	Pfister .	5,100,394	3/1992	Dudar et al. .
4,338,933	7/1982	Bayard et al. .	5,122,123	6/1992	Vaillancourt .
4,411,662	10/1983	Pearson .	5,135,489	8/1992	Jepson et al. .
4,417,890	11/1983	Dennehey et al. 604/256	5,154,703	10/1992	Bonaldo .
4,432,759	2/1984	Gross et al. .	5,158,554	10/1992	Jepson et al. .
4,432,765	2/1984	Oscarsson .	5,167,642	12/1992	Fowles .
4,439,193	3/1984	Larkin .	5,167,647	12/1992	Wijkamp et al. 604/281
4,457,749	7/1984	Bellotti et al. .	5,167,648	12/1992	Jepson et al. .
4,508,367	4/1985	Oreopoulos et al. .	5,171,234	12/1992	Jepson et al. .
4,511,359	4/1985	Vaillancourt .	5,188,620	2/1993	Jepson et al. .
4,512,766	4/1985	Vailancourt .	5,211,638	5/1993	Dudar et al. .
4,592,356	6/1986	Gutierrez .	5,273,533	12/1993	Bonaldo .
4,610,469	9/1986	Wolff-Mooij 285/260	5,290,254	3/1994	Vaillancourt .
4,617,012	10/1986	Vaillancourt .	5,344,414	9/1994	Lopez et al. .
4,645,494	2/1987	Lee et al. .	5,401,245	3/1995	Haining .
			5,411,499	5/1995	Dudar et al. .

U.S. Patent

Jul. 27, 1999

Sheet 1 of 19

5,928,204

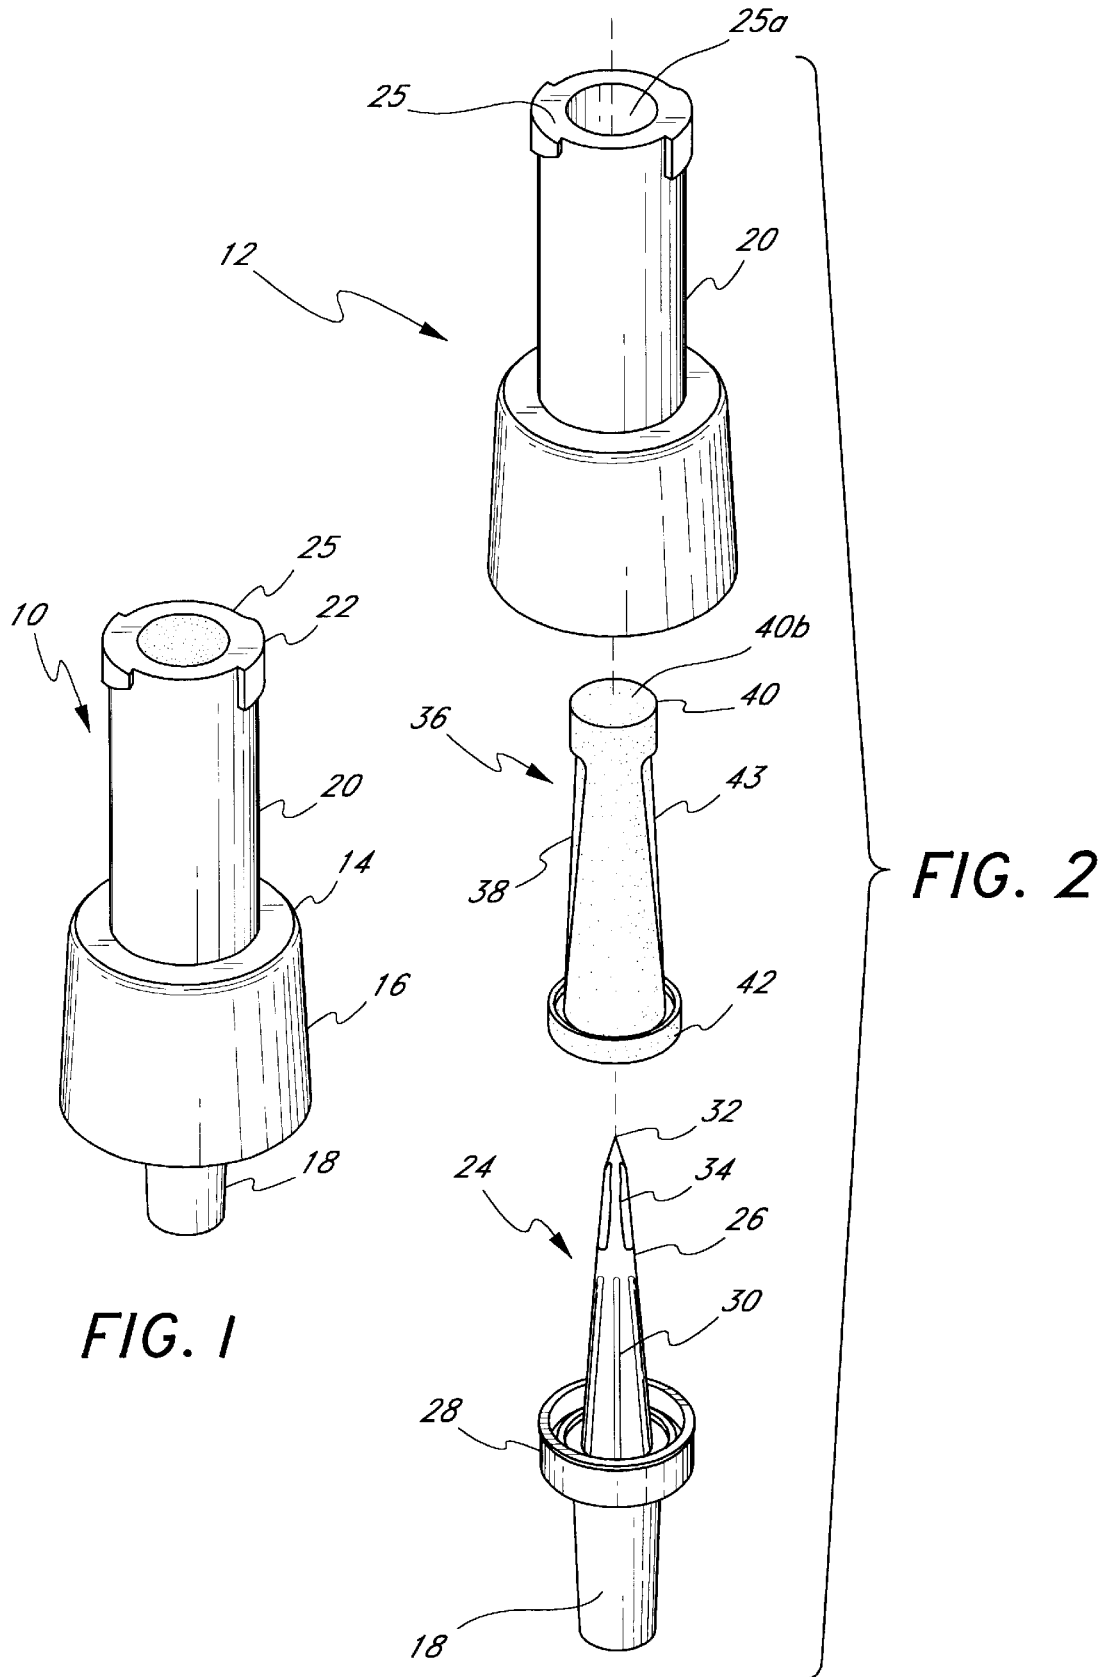

U.S. Patent

Jul. 27, 1999

Sheet 2 of 19

5,928,204

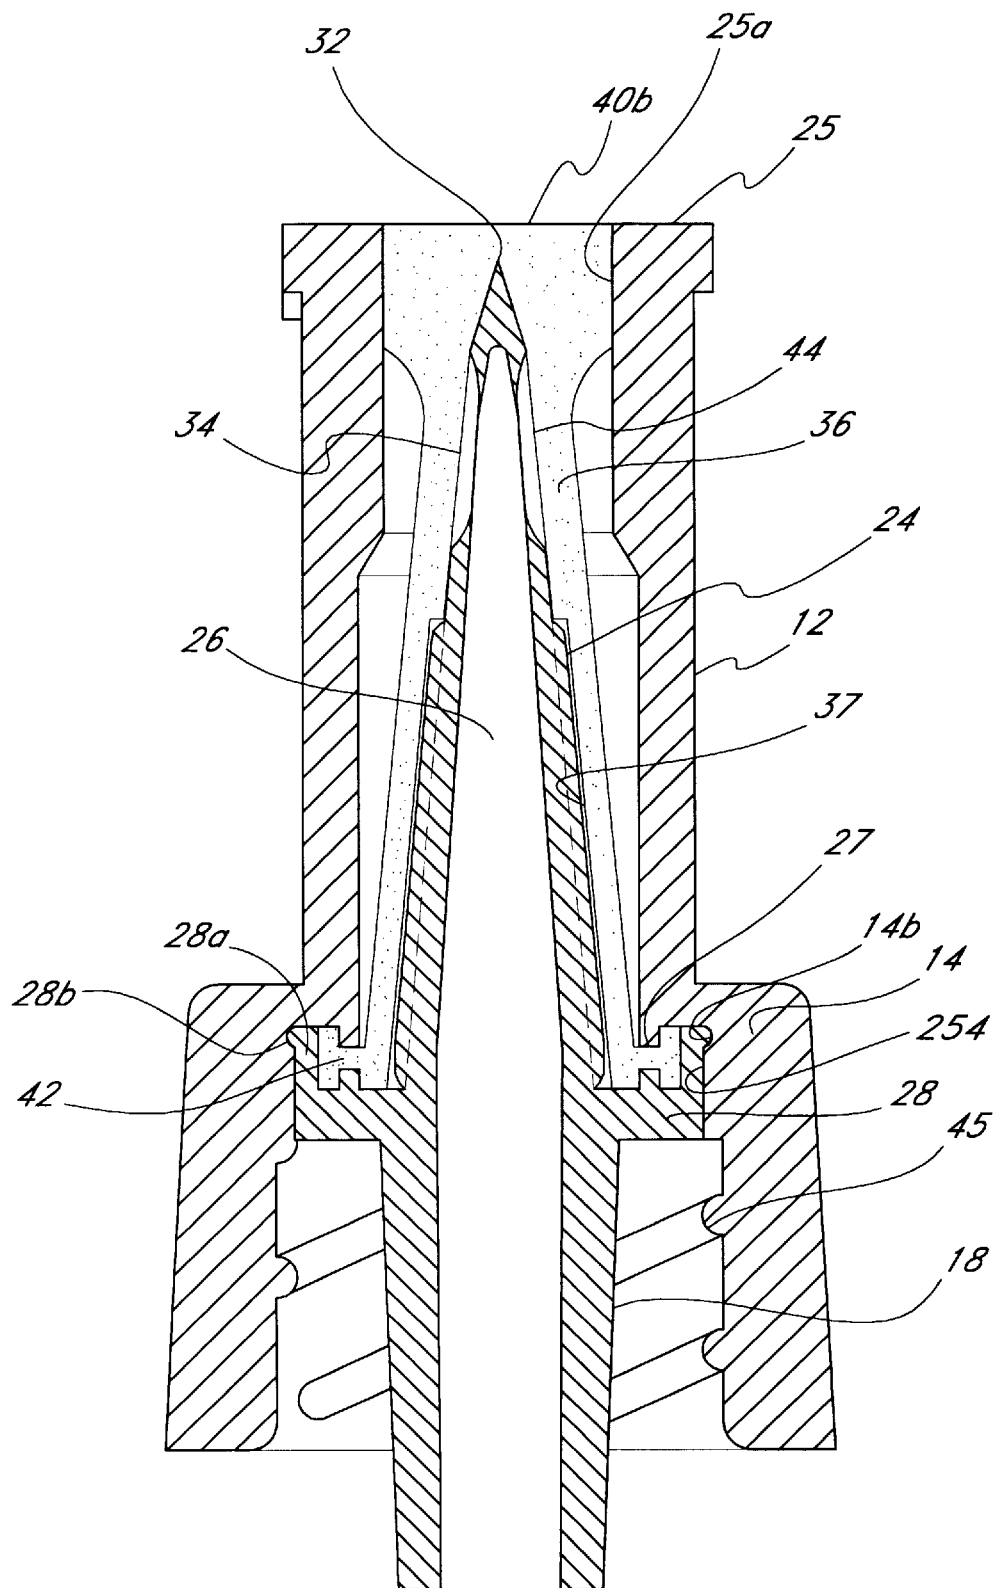


FIG. 3

U.S. Patent

Jul. 27, 1999

Sheet 3 of 19

5,928,204

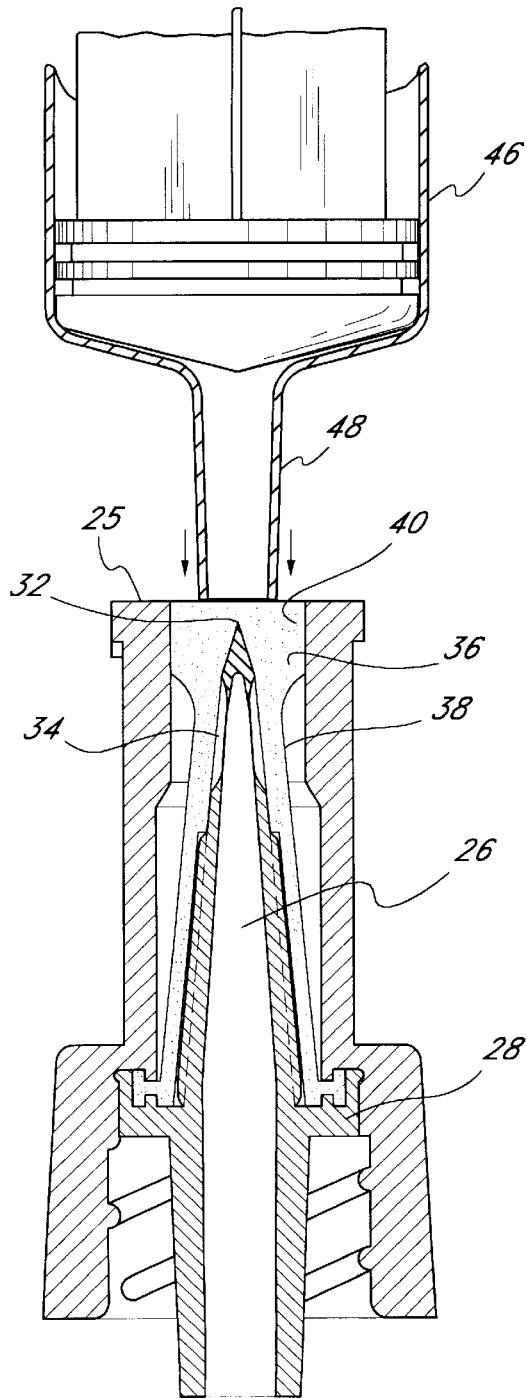


FIG. 4

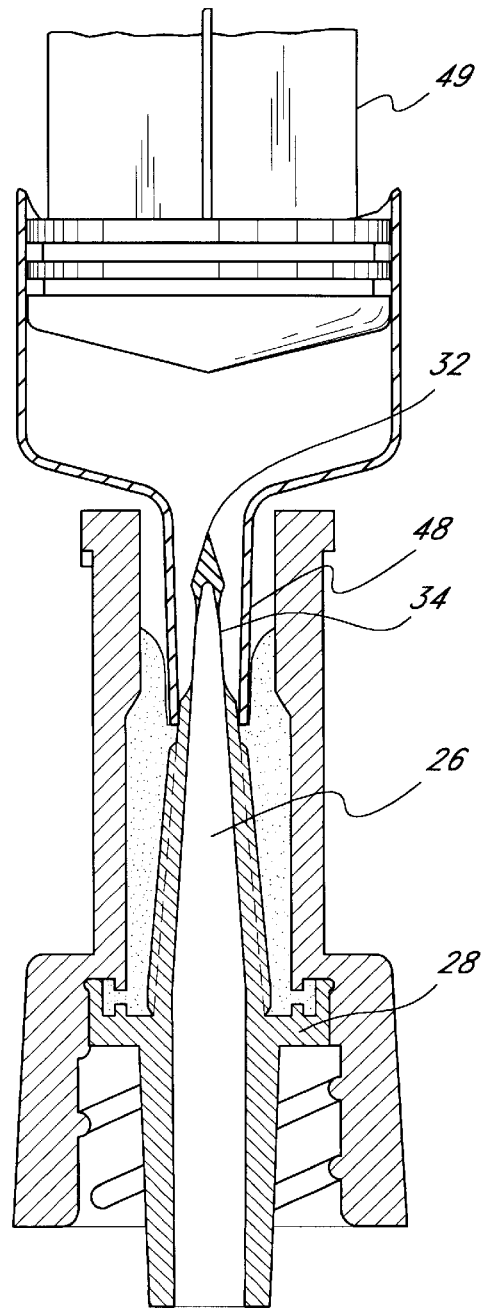


FIG. 5

U.S. Patent

Jul. 27, 1999

Sheet 4 of 19

5,928,204

FIG. 6

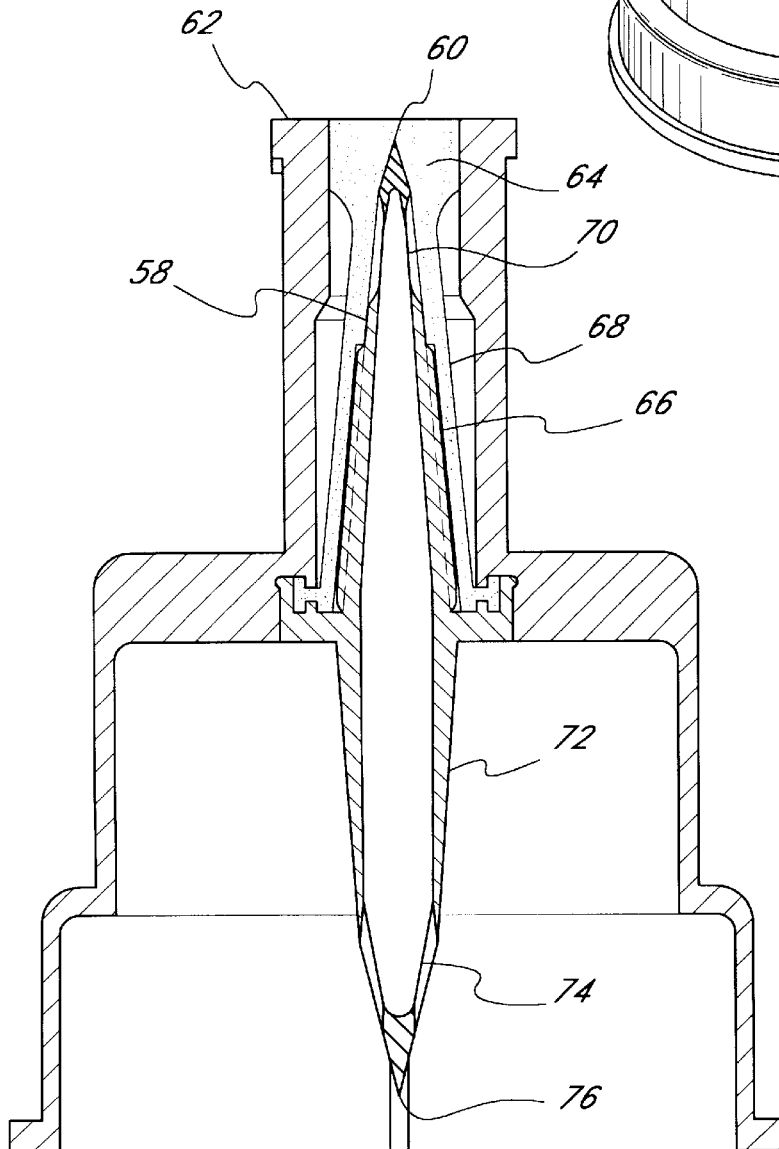
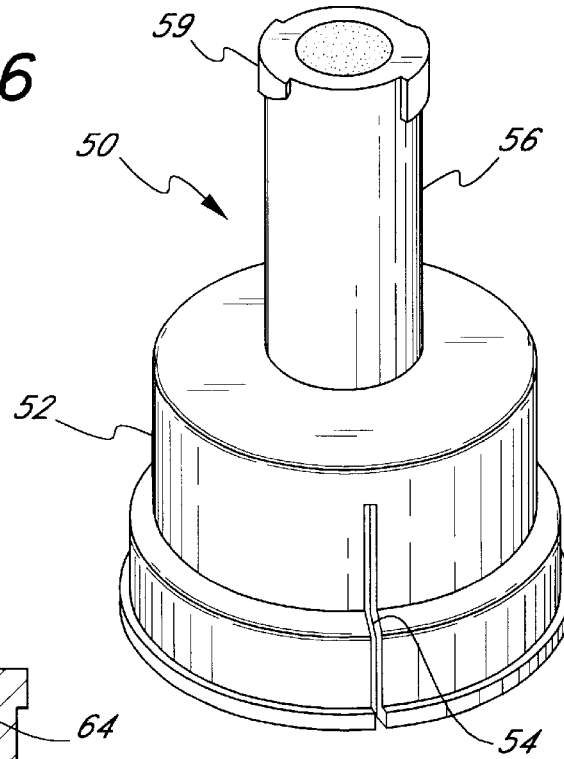


FIG. 7


U.S. Patent

Jul. 27, 1999

Sheet 5 of 19

5,928,204

FIG. 8

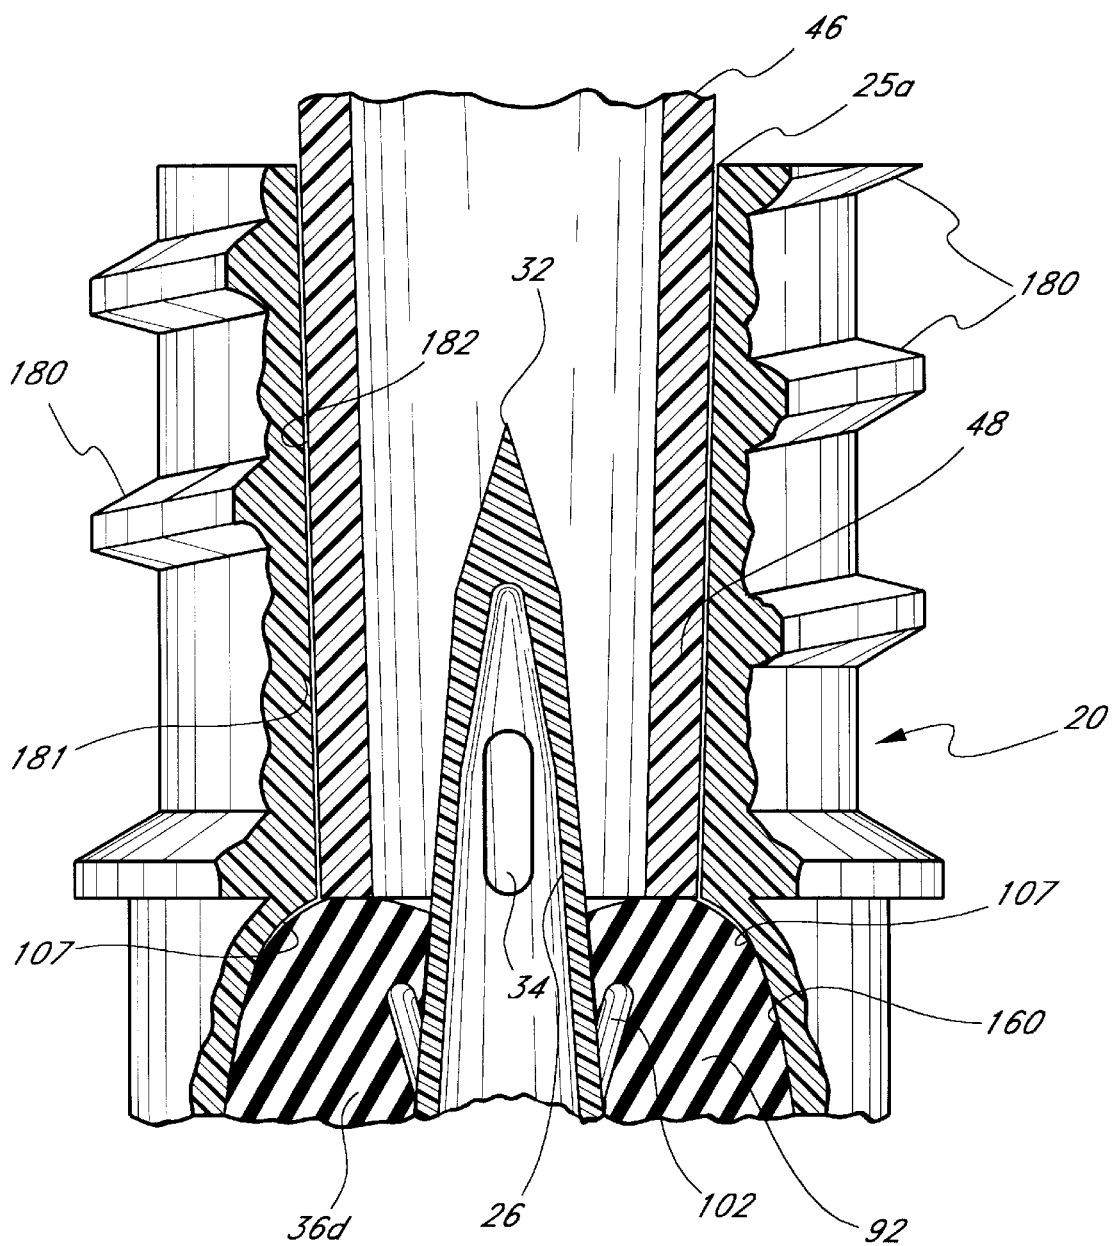

U.S. Patent

Jul. 27, 1999

Sheet 6 of 19

5,928,204

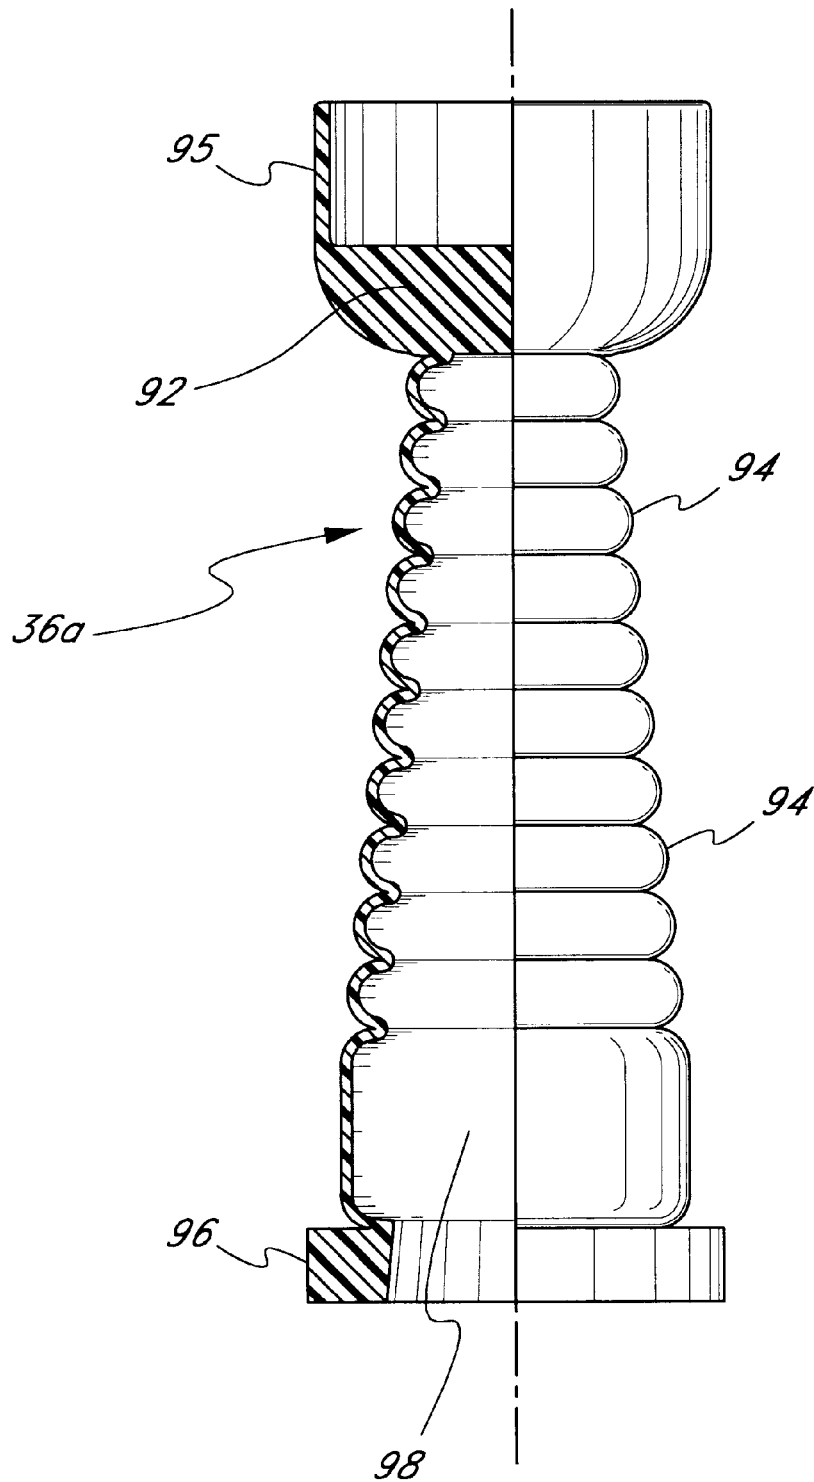


FIG. 9

U.S. Patent

Jul. 27, 1999

Sheet 7 of 19

5,928,204

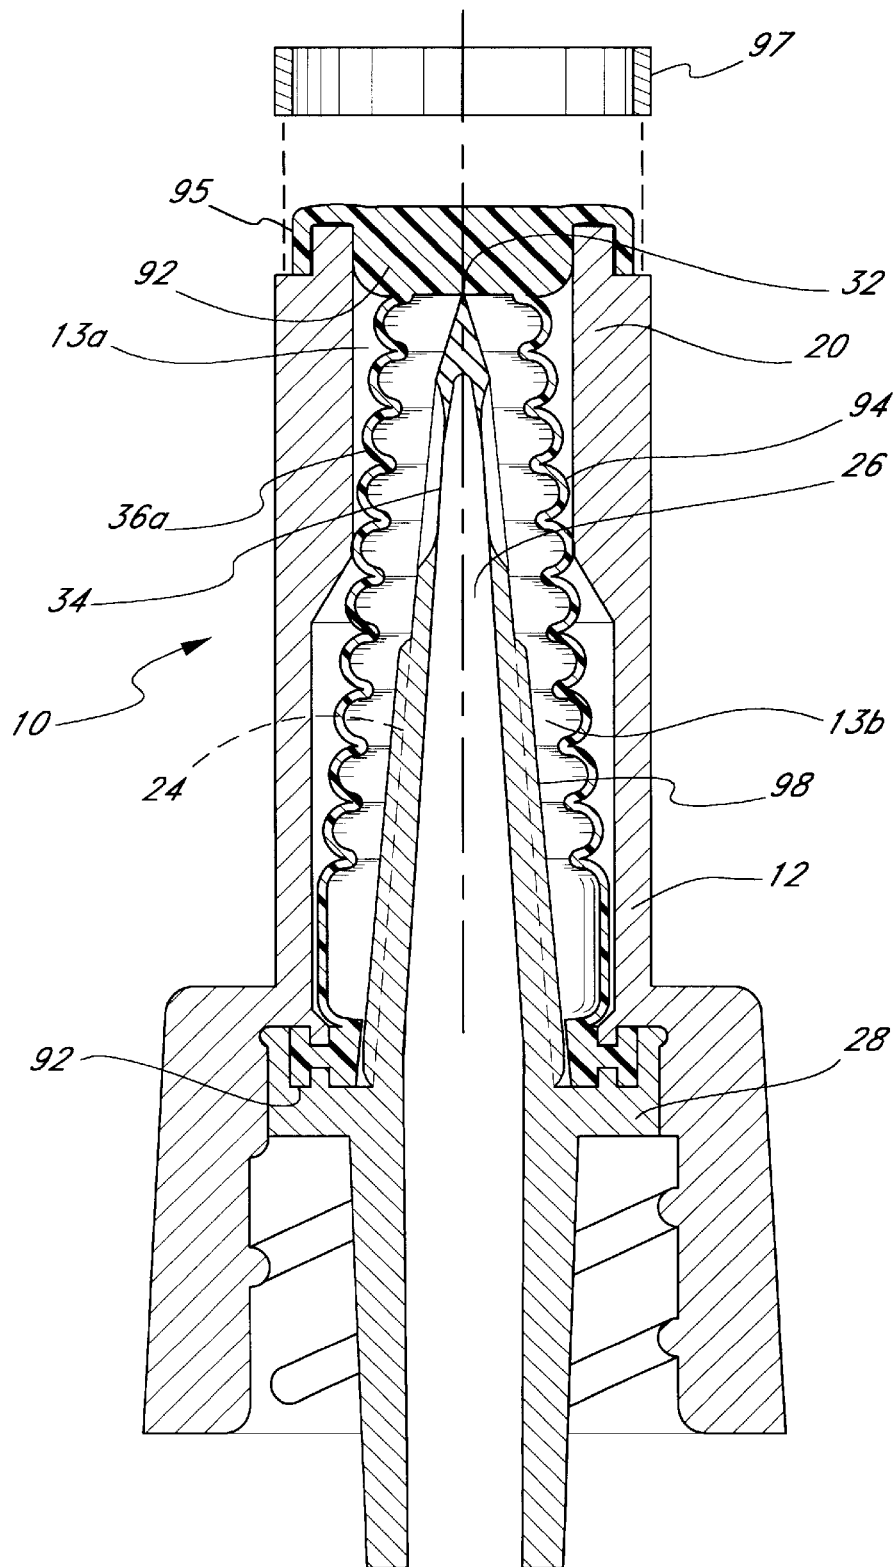


FIG. 10

U.S. Patent

Jul. 27, 1999

Sheet 8 of 19

5,928,204

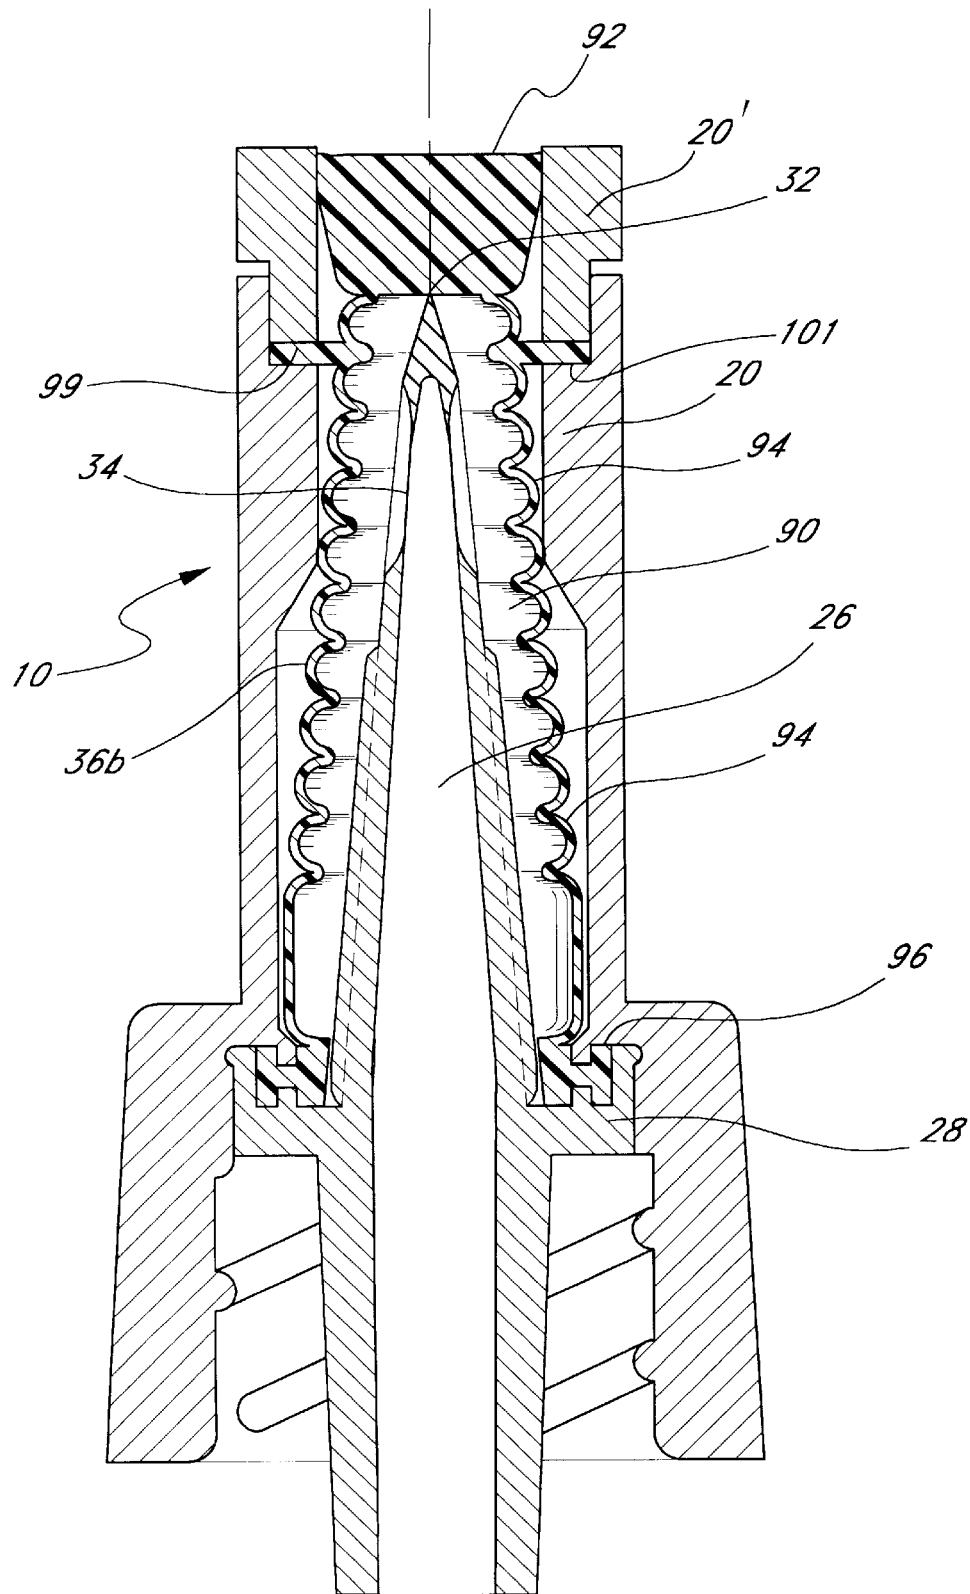


FIG. 11

U.S. Patent

Jul. 27, 1999

Sheet 9 of 19

5,928,204

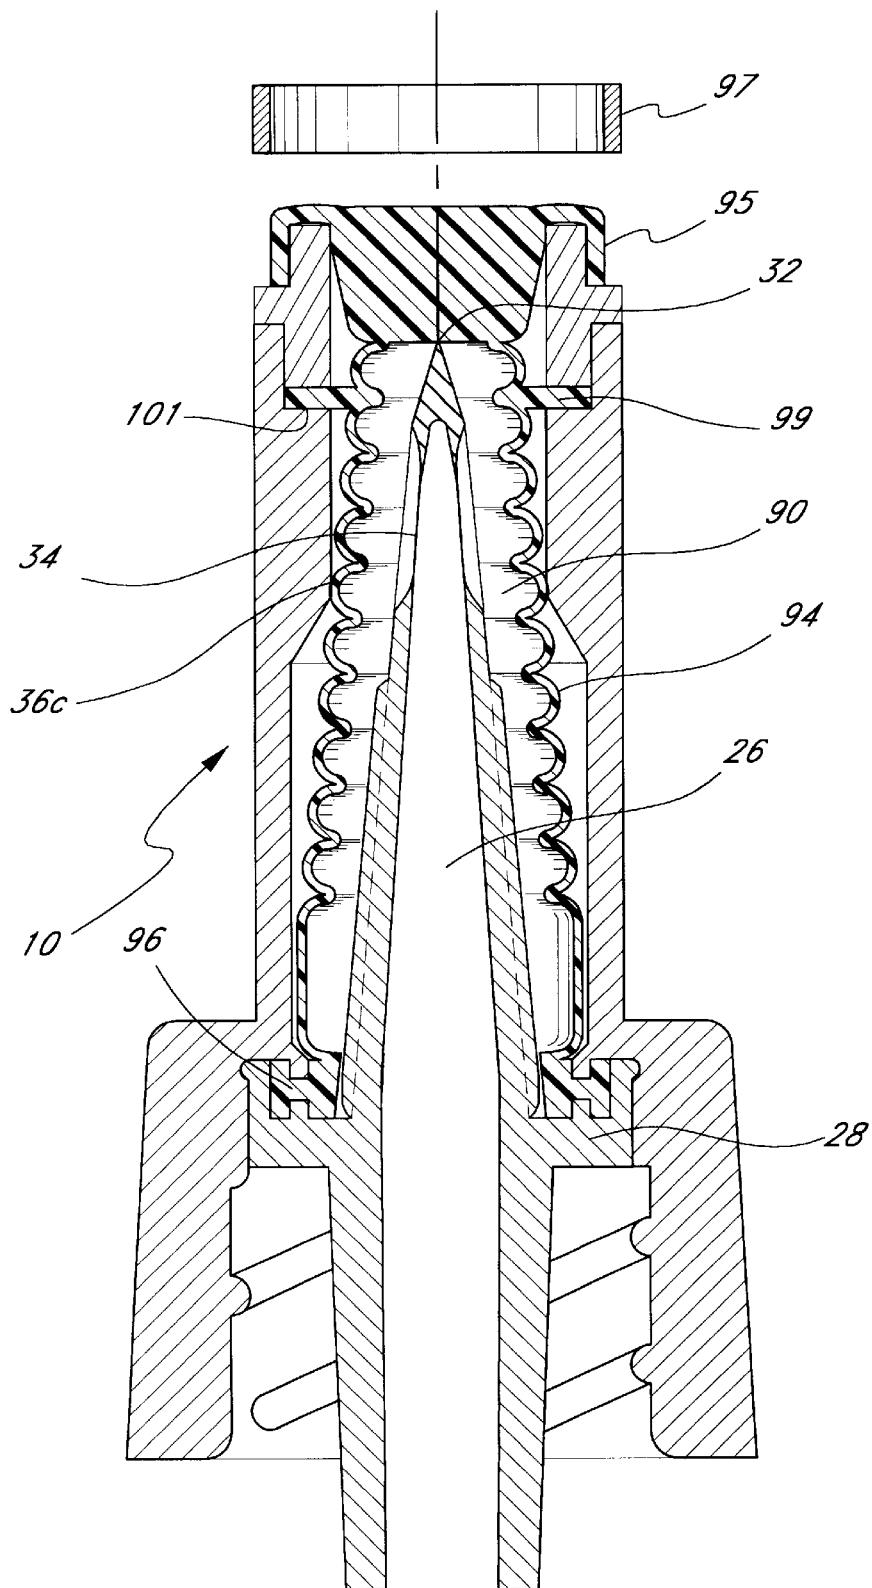


FIG. 12

U.S. Patent

Jul. 27, 1999

Sheet 10 of 19

5,928,204

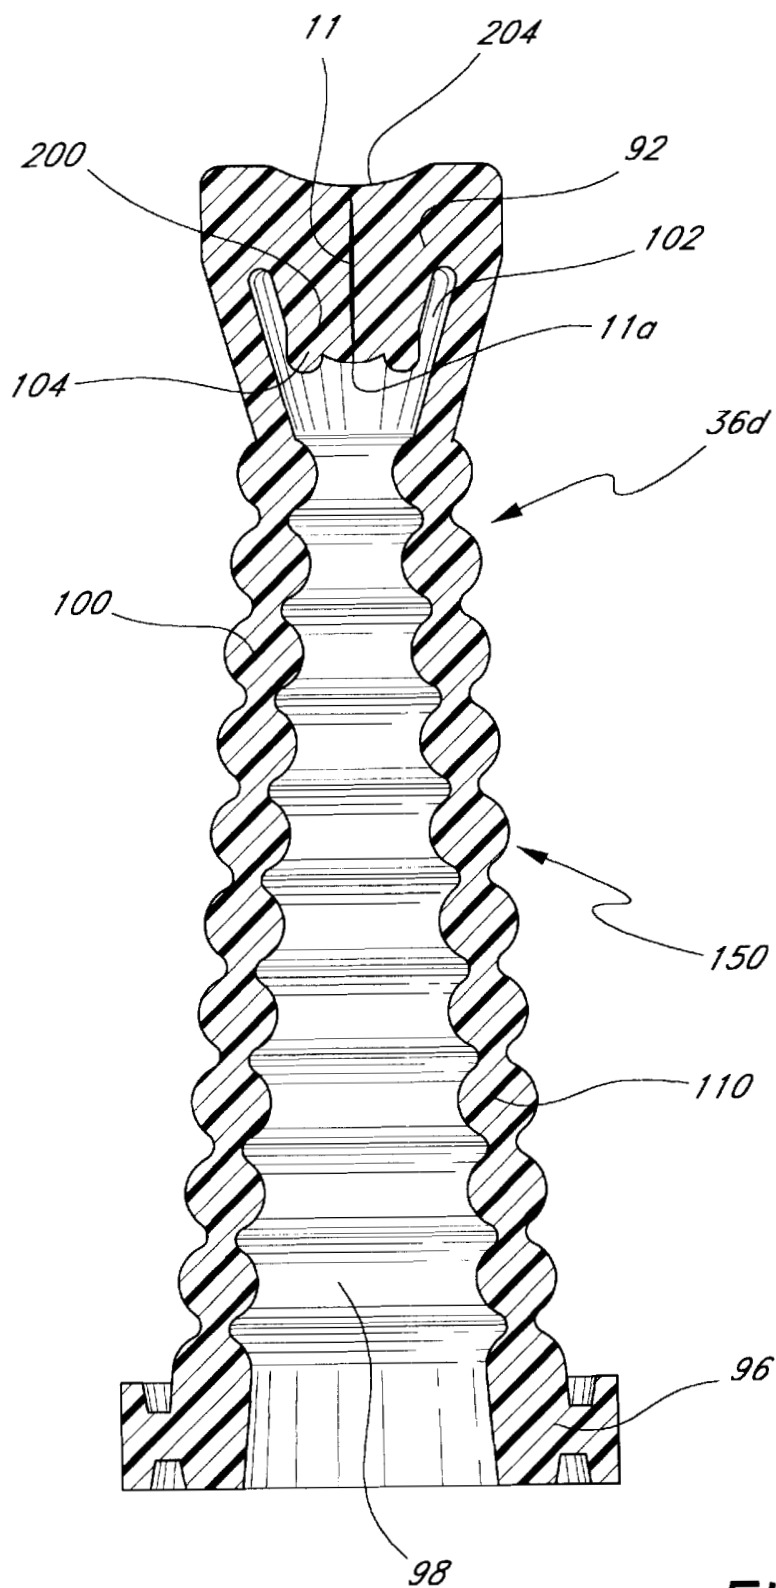


FIG. 13

U.S. Patent

Jul. 27, 1999

Sheet 11 of 19

5,928,204

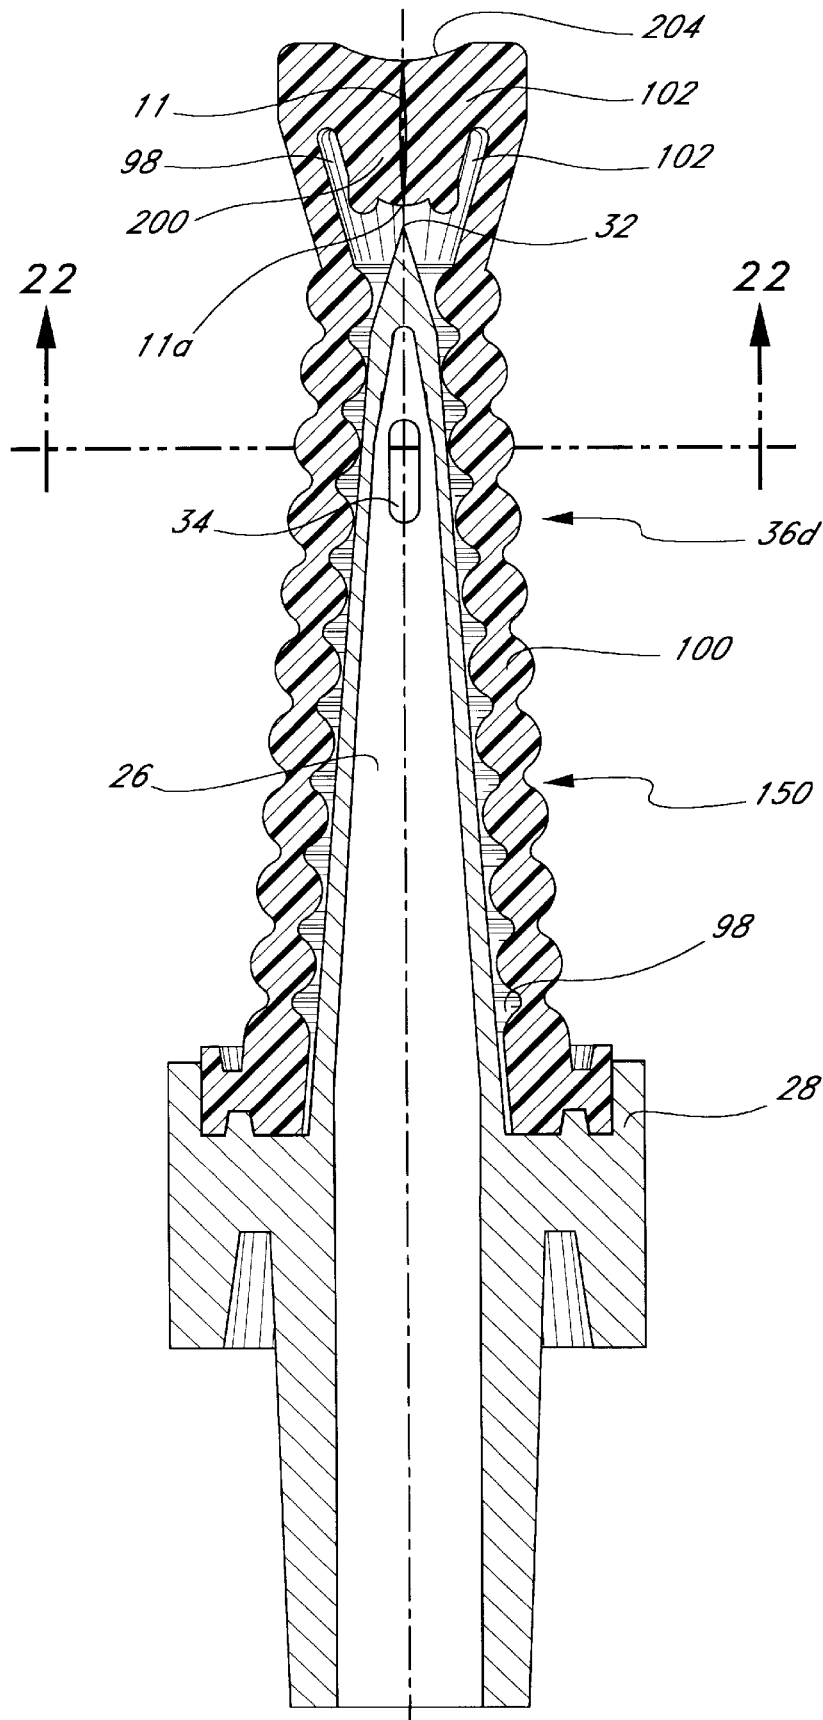


FIG. 14

U.S. Patent

Jul. 27, 1999

Sheet 12 of 19

5,928,204

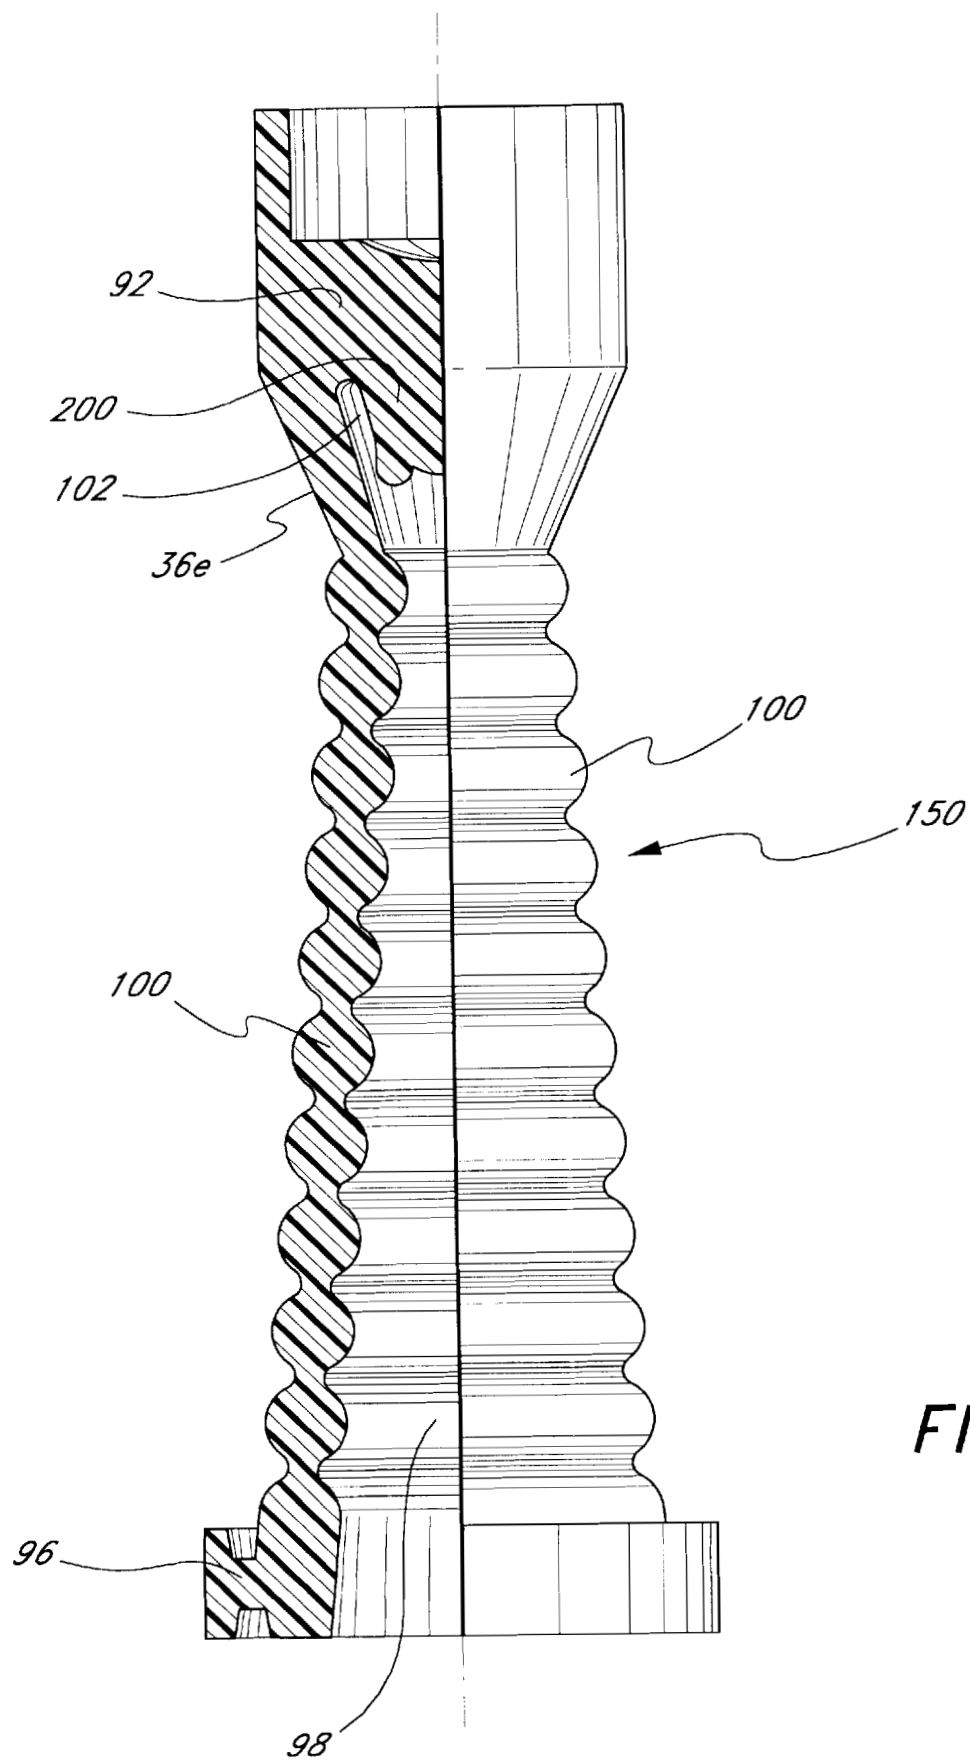


FIG. 15

U.S. Patent

Jul. 27, 1999

Sheet 13 of 19

5,928,204

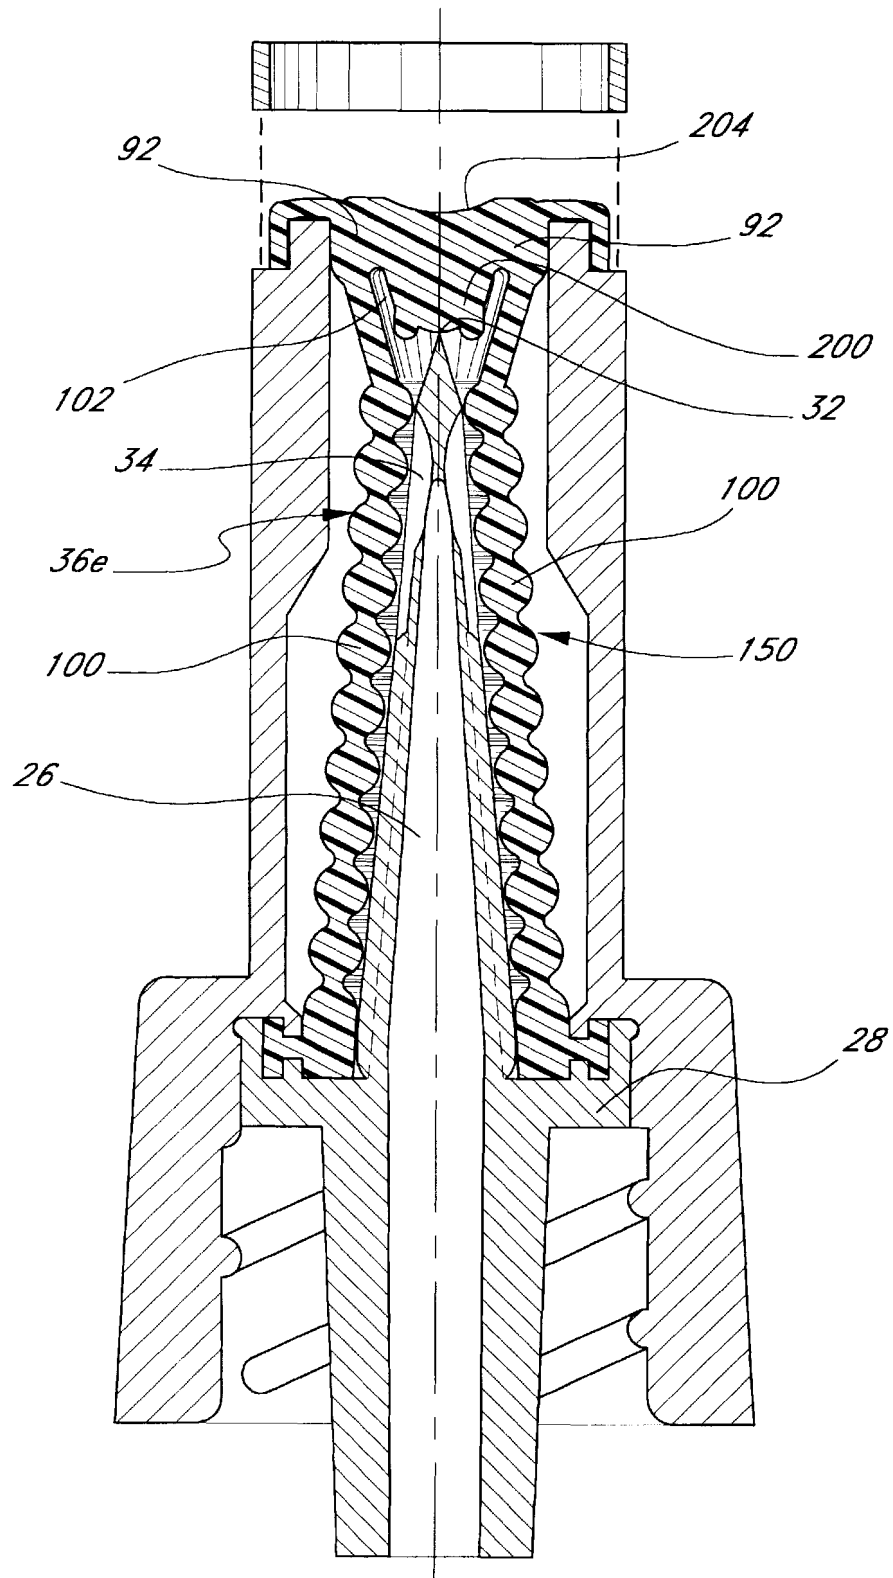


FIG. 16

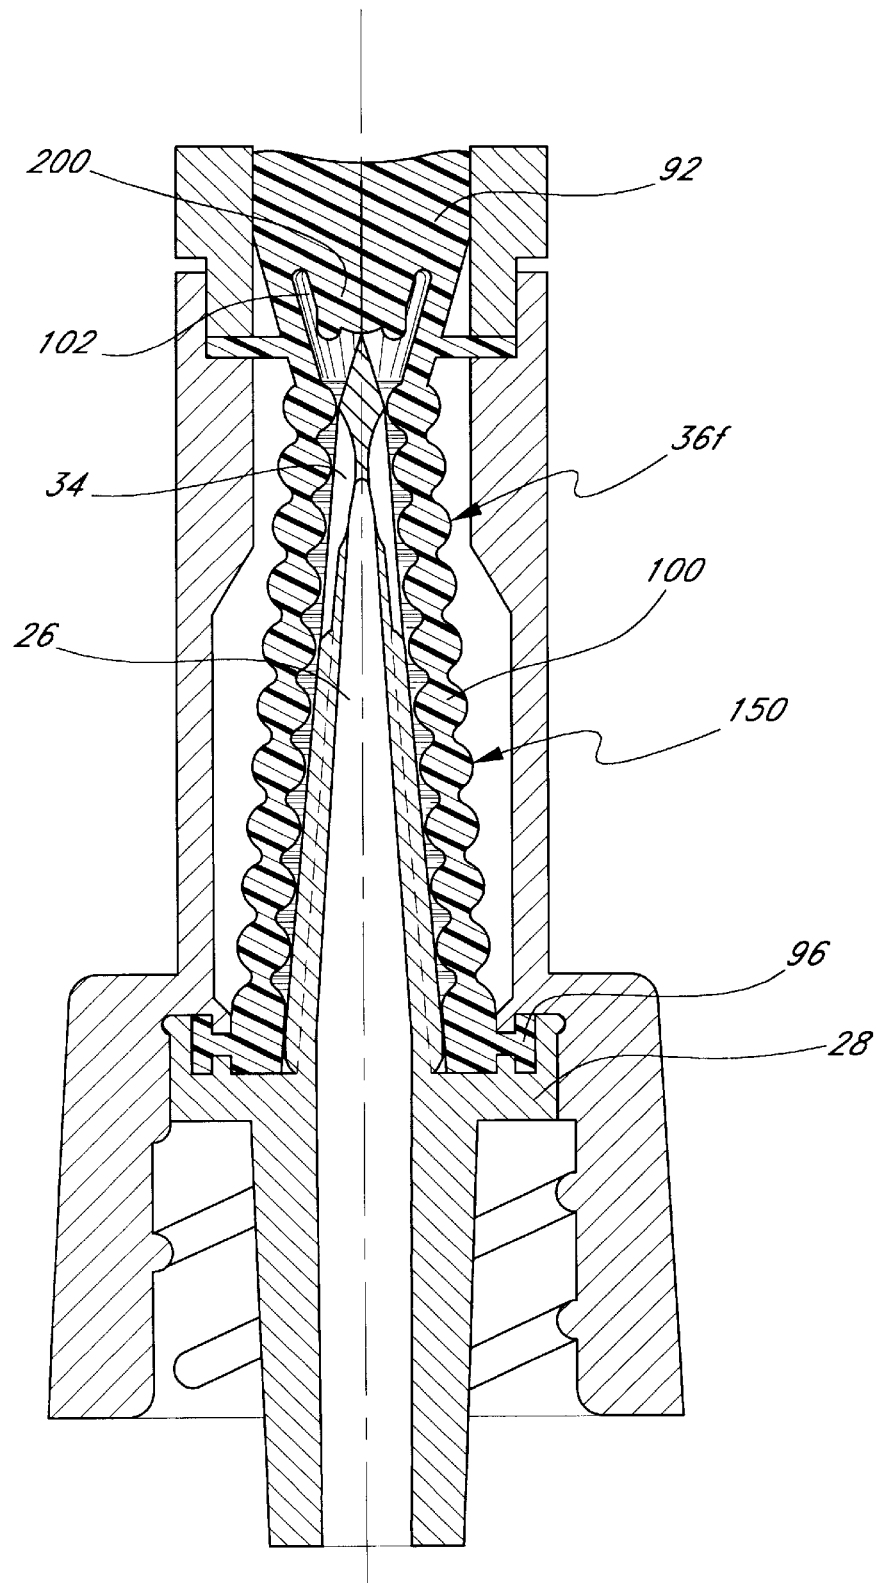


FIG. 17

U.S. Patent

Jul. 27, 1999

Sheet 15 of 19

5,928,204


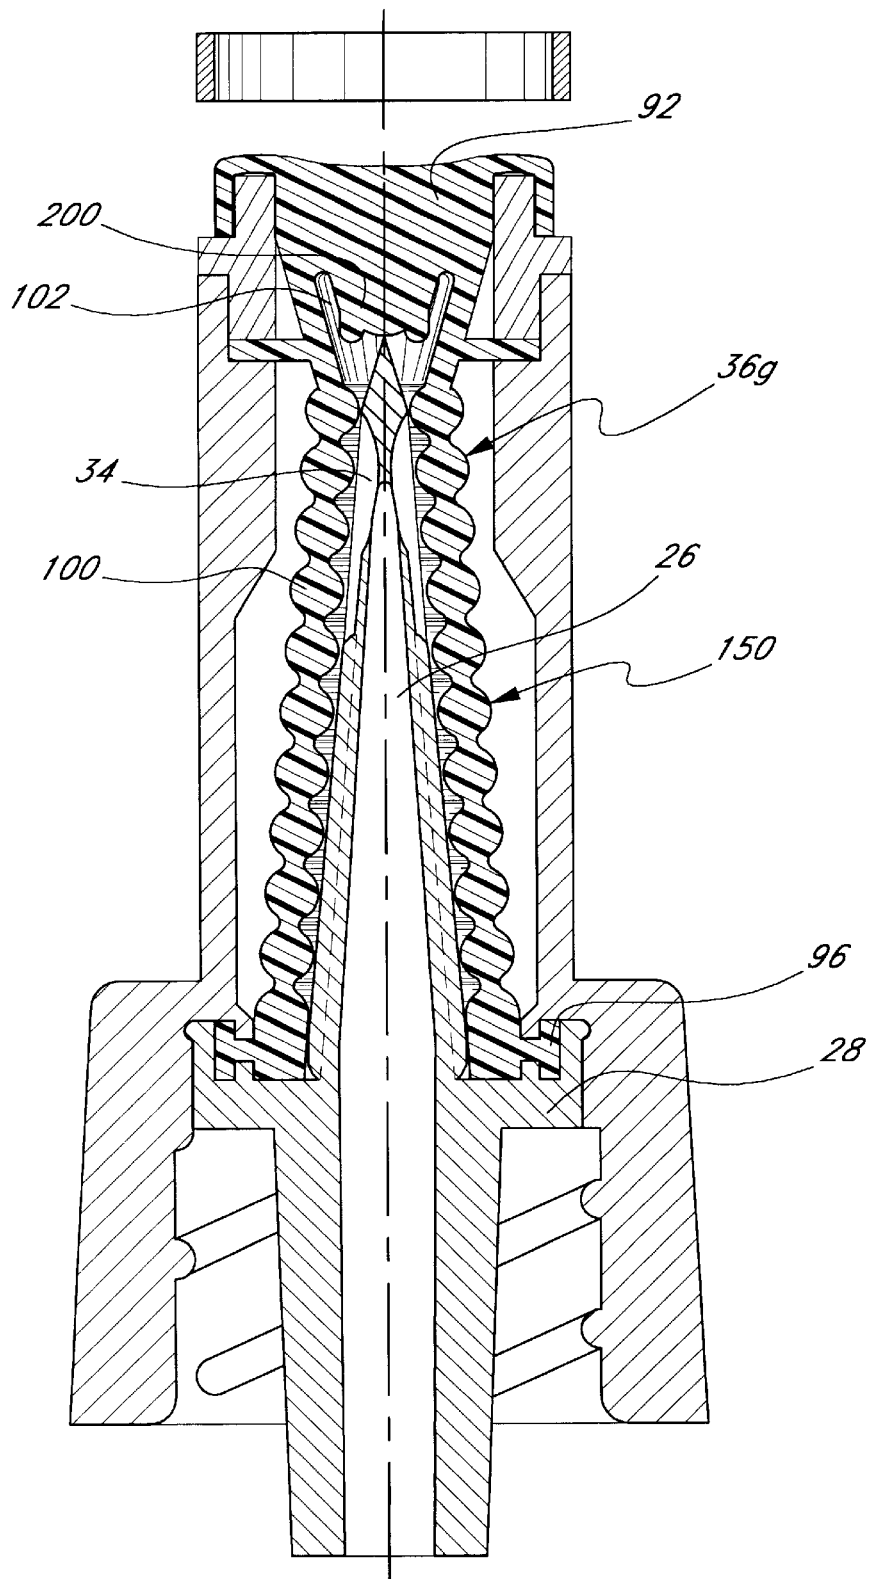


FIG. 18

FIG. 19

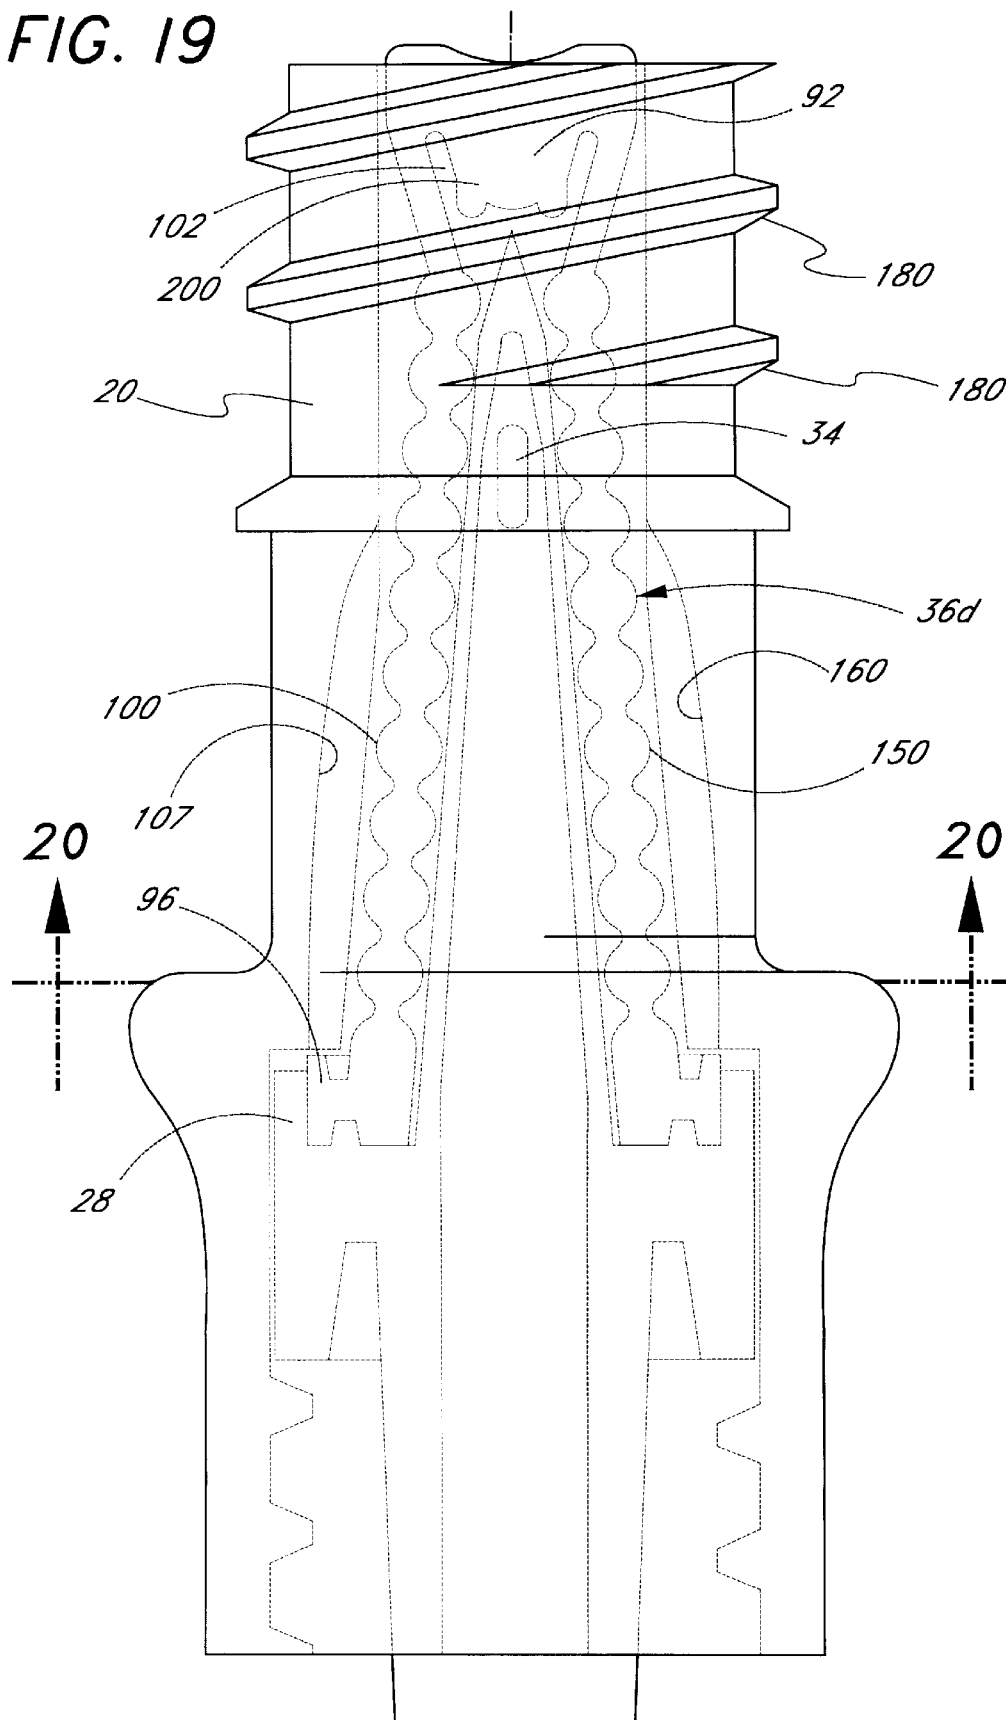

U.S. Patent

Jul. 27, 1999

Sheet 17 of 19

5,928,204

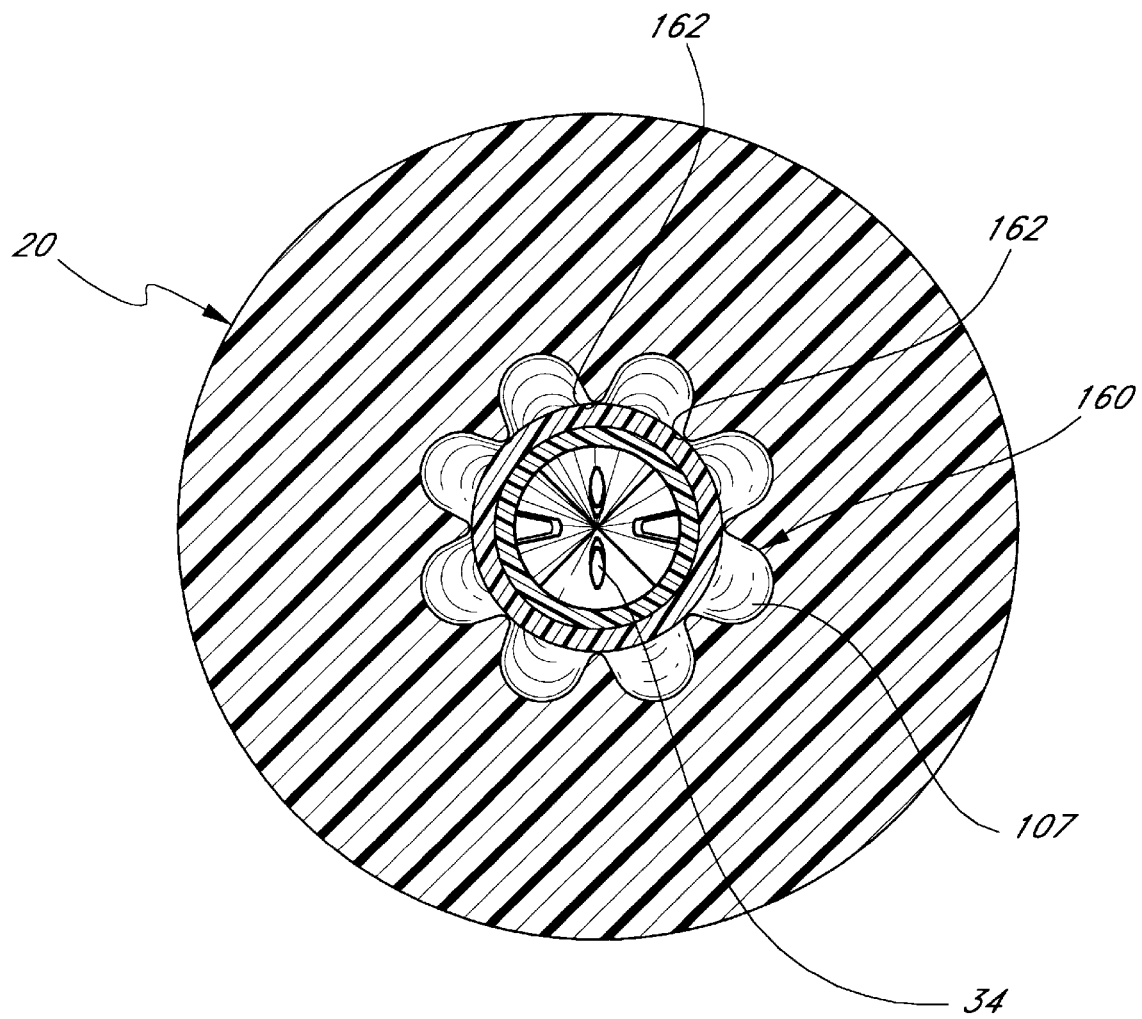


FIG. 20


U.S. Patent


Jul. 27, 1999

Sheet 18 of 19

5,928,204

FIG. 21

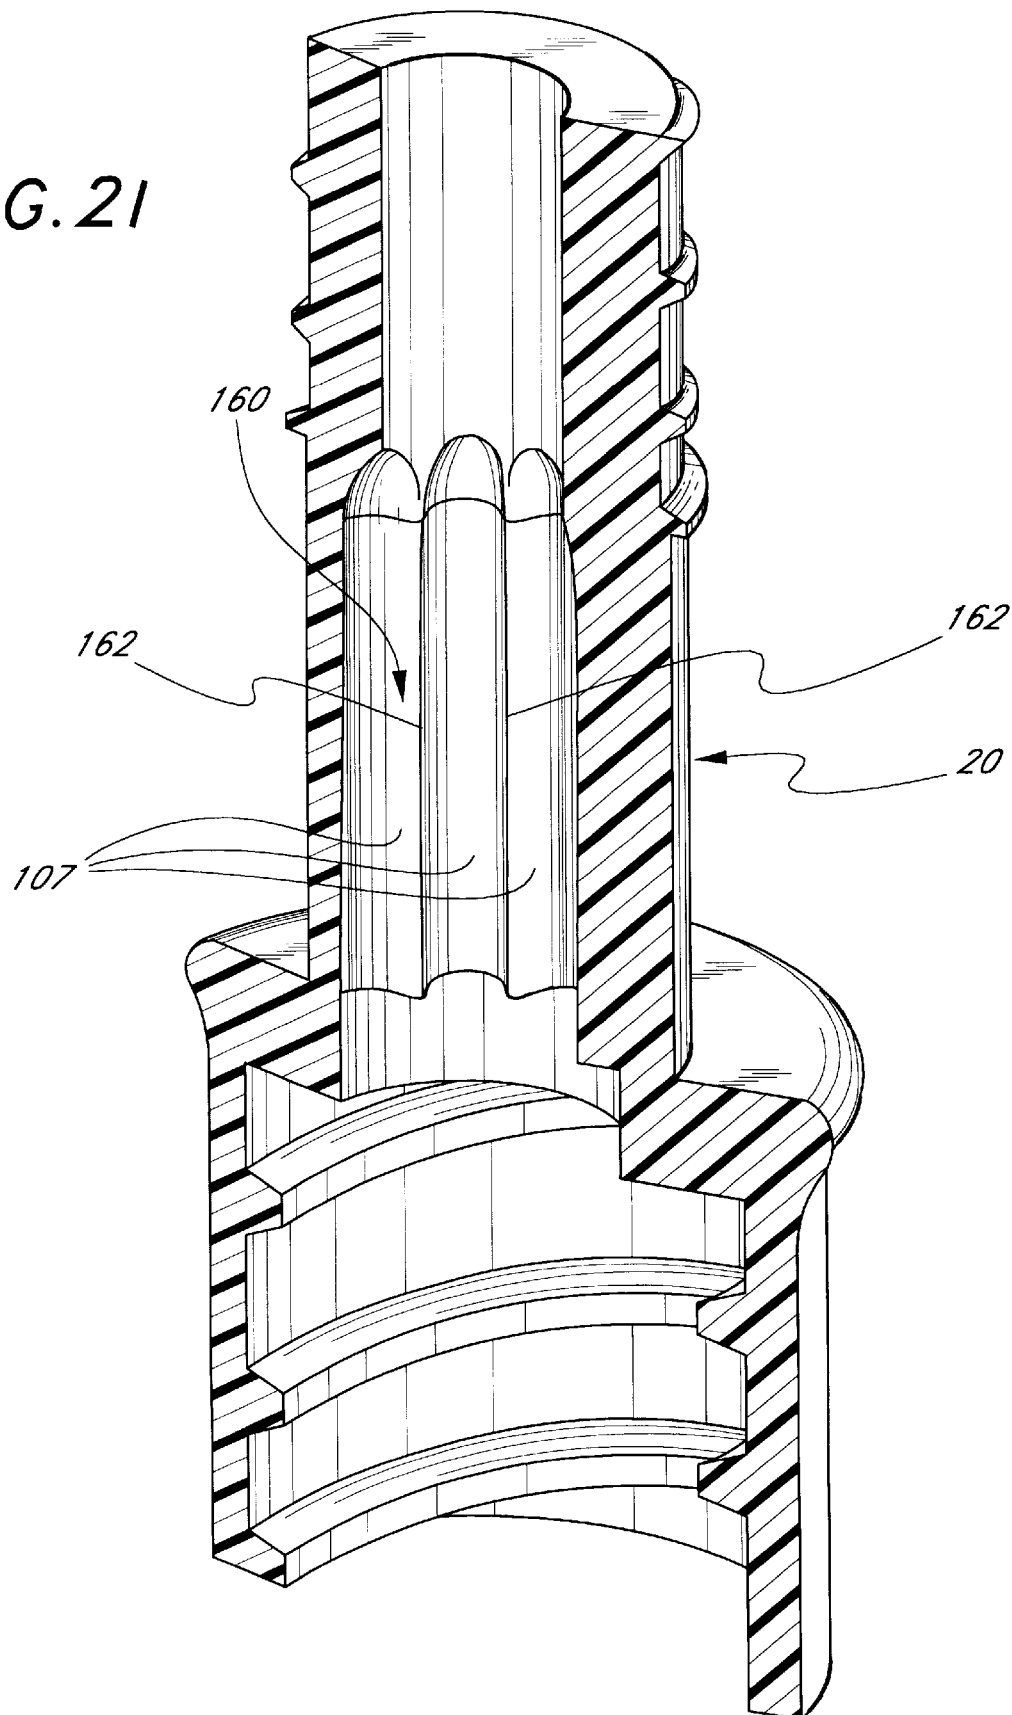

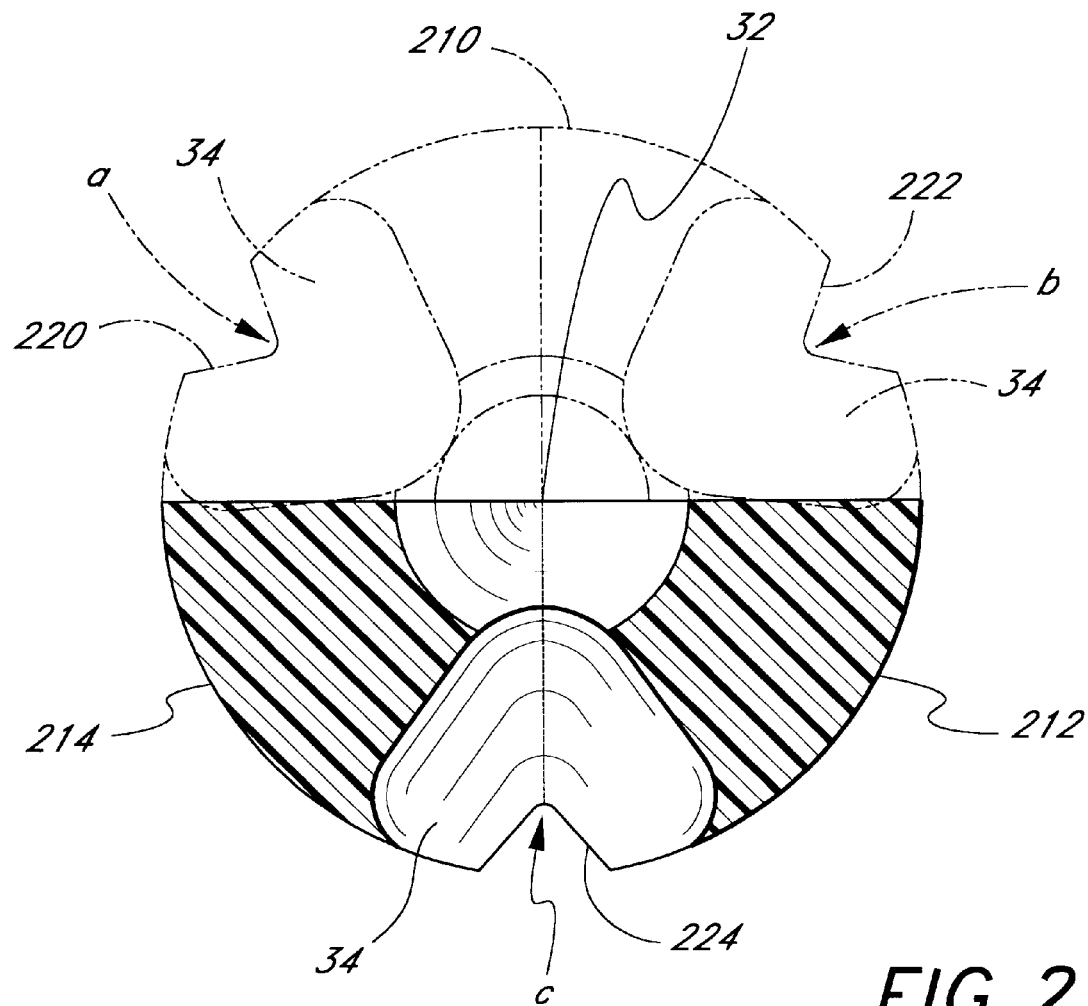

5,928,204

1

MEDICAL VALVE AND METHOD OF USE

This application is a continuation of U.S. patent application Ser. No. 08/334,846, filed Nov. 4, 1994 now U.S. Pat. No. 5,685,866 which is a continuation of U.S. patent application Ser. No. 08/096,659, filed Jul. 23, 1993 now U.S. Pat. No. 5,695,466, which is a continuation-in-part of PCT application Ser. No. PCT/US92/10367, filed Dec. 1, 1992, now abandoned, which is a continuation-in-part of U.S. patent application Ser. No. 07/813,073, filed Dec. 18, 1991, now abandoned.

BACKGROUND OF THE INVENTION**1. Field of the Invention**

This invention relates to a closed, patient access system which automatically reseals after administering medication using a standard medical implement that directly connects with the system without the need of any intermediary needles, caps or adaptors. A two-way valve eliminating dead space is used which includes a seal which, upon being compressed by the medical implement, is pierced to open the valve and reseals upon being decompressed, maintaining a fluid tight seal even at high pressures and after repeated uses.

2. Background Discussion

The manipulation of fluids for parenteral administration in hospital and medical settings routinely involves the use of connectors and adaptors for facilitating the movement of fluids between two points. Most fluid connectors and adaptors employ needles to pierce a septum covering sterile tubing or to pierce the septum of a medicament container of fluid. Fluid then passes from the container or fluid filled tubing into a syringe or second set of tubing. These connectors and adaptors often have mechanical or moving parts. Since the ready passage of fluids through the connectors and adaptors is often critical to patient survival, it is imperative that the connectors and adaptors function reliably and repeatedly. Adaptors and connectors that malfunction during use may be life-threatening. The more mechanical or moving parts such as springs and diaphragms, the more likely that they will function improperly. Improper functioning can result in the introduction of air embolisms into a patient. Thus, the fewer the mechanical parts, the more these connectors can be relied on and the better they will be accepted by the medical community.

Many connectors or valves, especially those employing several mechanical components, have a relatively high volume of fluid space within them. This "dead space" within the device prevents accurate introduction of precise fluid volumes and provides an opportunity for contamination upon disconnection of the device. Connectors and adaptors often include valves that permit or interrupt the flow of fluid along the course of fluid travel. Several of those commonly in use employ metal needles to puncture sterile seals. Such connectors are generally designed to accommodate fluid flow in one direction. This means that the fluid line must have connectors and tube aligned in complementary directions. These connectors often require further manipulation if, for example, the valve is inadvertently assembled in a direction that will not facilitate fluid flow. These manipulations increase handling, thereby increasing both the risk of contamination and the amount of time required to establish the fluid connection.

Metal needles employed as part of connector devices increase the risk of puncture wounds to the user. The needles used in these devices often have through-holes placed at the tip of the needle. Connection of the valve with a flow line

2

involves piercing the needle through a sealed septum. Through-holes placed at the needle tip can core the septum and release free particulates into the flow line. Such an event can prove fatal to a patient. Such through-holes may also become clogged easily with material from the septum.

Reusable connectors and adaptors are preferred for medical applications since components must often be added or removed from a fluid line connected to a patient. Reusable connectors, however, are difficult to keep sterile. Sometimes caps are employed to cover the connector to keep it sterile. Frequently, these caps are lost, or simply not used because they are not readily available when needed.

A closed, patient access system that is easy to use and employs only a valve device in communication with the patient that need not be capped or interconnected with the medical implement through a needle or adaptor, is swappable, is sufficiently durable to maintain its function after several manipulations, and maintains a fluid-tight seal at high pressures, would be of great benefit to the medical community.

SUMMARY OF THE INVENTION

The valve of this invention has several features, no single one of which is solely responsible for its desirable attributes. Without limiting the scope of this invention as expressed by the claims which follow, its more prominent features will now be discussed briefly. After considering this discussion, and particularly after reading the section entitled, "DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS," one will understand how the features of this invention provide its advantages, which include safety, reliable and repeatable performance, elimination of dead space, simplicity of manufacture and use, and employment of a valve that is swappable after use to provide sterility and has a fluid-tight seal at high pressure.

This invention is a closed, patient access system which automatically reseals after administering medication using a medical implement that directly connects with the system without the need of any intermediate needles, caps or adaptors. A two-way valve is employed utilizing a reusable seal that may be repeatedly pierced by an enclosed, protected, non-metallic spike rather than an exposed metal needle. The valve facilitates fluid, particularly liquid, transfer while maintaining sterility. The valve is easy to use and is capable of locking in place. After use, the valve is swabbed in the conventional manner with a suitable substance to maintain sterility. The design of the valve avoids accidental needle sticks. As will be discussed in detail below, the valve is useful as a medical connector or adaptor to enable liquid flow from a sealed container.

The first feature of this invention is that the valve has a body including wall structure defining an internal cavity having a proximal end and a distal end. The cavity has an open space into which the seal is pushed, and preferably has a plurality of radial indentations in the wall structure that are adjacent the seal to accommodate the expansion of the seal upon compression. The proximal end has an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through the delivery end. In most applications, the delivery end of the implement is tapered, and the wall structure adjacent the opening is tapered inward so that the wall structure and the tapered delivery end fit snug against each other upon insertion of the delivery end into the opening. The proximal end of the cavity preferably is adapted to fit snug with an ANSI (American National Standards Institute, Washington, D.C.) standard end of the

5,928,204

3

medical implement. Typically, the implement is a syringe, a connector or inlet/outlet of an IV set, or any one of a wide variety of conduits used in medical applications.

The second feature is that the spike has a tip with at least one hole located at or near the tip, and a passageway in communication with the hole that allows fluid to flow through this hole. The spike is seated inside the cavity such that the tip is inward of the proximal end and is enclosed within the cavity. Preferably, the hole is in a side of the spike adjacent the tip and is elongated, having a size of 18 gauge or greater. The tip may be sharp or slightly rounded. More than one hole is desirable for many applications, and three, symmetrically located holes inward of the proximal end are preferred. The spike may include at least one rib which allows air to enter a space between the seal and the spike, thereby facilitating the sealing of the opening when the implement is removed. The spike may have a substantially conical shape, and the seal has a complementarily, substantially conical shaped cavity within it conforming to the shape of the spike. The spike is disposed within this conical cavity and the seal covers the tip. The tip may be imbedded in the proximal end of the seal or withdrawn into the conical cavity. Preferably, the tip of the spike has a plurality of facets which meet within a recess. The preferred spike should be able to penetrate the seal repeatedly without tearing the seal. Rough edges at the tip may present a tear problem. During injection molding of the preferred plastic spike, facets of the tip will abut along a "parting line," and could form a rough edge which may tear the seal. This problem is avoided where the parting line is buried in a recess. Any rough edge at this parting line is disposed within a recess, so the seal material moves over the recess and does not contact the rough edge.

The third feature is that the resilient seal is adapted to be moved into a compressed state upon insertion of the tip of the medical implement into the opening and returns to a decompressed state upon removal of the tip. The seal in the decompressed state has a section which fills essentially completely a portion of the cavity adjacent the opening. The seal section bears against the wall structure near the opening to seal the opening. In the compressed state, the seal section is pushed by the delivery end of the medical implement away from the opening and into the cavity. A fluid tight seal is maintained between the seal section and the wall structure as the seal is moved into the compressed state. The seal section bears against the wall structure as the seal is moved inward into the cavity by the tip of the medical implement. And most importantly, the delivery end and the seal are adapted to engage so that when the tip of the spike pierces the seal there is essentially no dead space between said delivery end and the seal. Consequently, a predetermined dosage amount of medication is transferred in its entirety to the patient using this invention, with none to the prescribed amount being collected in dead space in the valve. The delivery of an exact amount of medication may be critical in some situations when chemotherapeutic agents are being administered or small children are being treated.

A fluid tight seal is maintained over repeated opening and closing of the valve, and the seal has on its external surface a recess which provides an air pocket to facilitate the movement of the seal. Preferably, the seal presents an essentially flush surface with the proximal end of the cavity. In one embodiment, the proximal end of the seal is substantially flat, the seal is made of a material having a hardness of from 30 to 70 Shore units such as, for example, a silicone polymer. The seal may include a cup-like flange adapted to engage the body near the proximal end of the cavity. A preferred embodiment of the seal comprises a series of

4

O-ring elements stacked together and connected to form a unitary structure. The O-ring elements have increasing diameters, with the smallest diameter element being adjacent the proximal end of the cavity. The proximal end of the seal may be precut to form a tiny orifice therein that allows the tip of the spike to pass therethrough easily upon compression of the seal. Preferably, the proximal end of the seal has a truncated conical shaped segment disposed within the cavity. The seal may also have a centrally located, anti-vacuum, saucer like depression therein, which does not interfere with the ability of the exposed, proximal end of the seal being swabbed when desired.

The fourth feature is that the body and spike are two separate components of the valve that are securely attached to each other by assembly of, and interlocking, of the body and spike. The body has a first locking element near the distal end of the cavity, and the spike has a second locking element adapted to interlock with said first locking element upon assembly. The seal has a lip extending beyond the distal end and positioned between the first and second locking elements so that, upon assembly, the lip is compressed between the locking elements to provide an essentially fluid tight seal upon interlocking.

The fifth feature is that the medical valve includes a support member connected to the spike which seals off the distal end of the cavity. The support member may have a Luer-Lock type connector element that enables the valve to be removably attached to, for example, a fluid line connected to a patient. The support member may also be in the form of an adaptor that enables the valve to be removably attached to a fluid dispenser or container. When used to dispense fluids from a container, the spike has a pair of opposed tips, respectively at the distal and proximal ends of the spike. The tip at the distal end of the spike pierces a cover member which seals the container. A radial slit on the adaptor enables it to deform reversibly sufficiently to fit snugly onto said container.

The sixth feature is that the seal has a proximal end including a pressure responsive element disposed on an inner surface of the seal adjacent the opening. The pressure responsive element in the decompressed state closes any orifice in the seal at the proximal end of the seal to provide an essentially fluid-tight seal while in the decompressed state. The pressure responsive element enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve is connected to a patient's artery. The valve of this invention will remain closed even when the pressure inside the valve is above 6 pounds per square inch (psi), and it can withstand pressures above 30 psi. Typically, the pressure responsive element is a section of the seal having an entryway into a precut orifice. This section has a substantially cylindrical configuration and is surrounded by an annular space which is filled with pressurized fluid. The center of the member and the annular space are coaxial with the entryway to the orifice. The pressurized fluid fills the annular space to apply pressure that compresses the cylindrical section to tightly close the entryway to the orifice. Preferably, the pressure responsive element has an anti-tear element.

In accordance with this invention, a known, prescribed, predetermined amount or dosage of medication may be transferred from the remote source to the patient directly, so that essentially none of said predetermined amount is collected in dead space in the valve. In other words essentially all the prescribed dosage is received by the patient and not lost in the valve. Thus, this invention also includes a method

5,928,204

5

of transferring fluid from a remote source to a patient. This invention also includes transfer of fluid from the patient to a remote source. This is possible because the valve of this invention provides two-way communication. The fluid is transferred to the patient by applying pressure the fluid as it passes through the implement so that the pressure applied to the fluid is greater than the pressure of fluid in the patient, enabling transfer from the remote source to the patient. To achieve transfer of fluid from the patient to the remote source, the pressure of fluid in the patient is greater than the pressure at the remote source, causing fluid to flow from the patient to the remote source. This invention also includes a method of transferring fluid in a container having an open mouth covered by a cover member which seals the open mouth. The fluid is caused to flow from the container through the passageway by creating a differential in pressure. Preferably, the valve has an adaptor having a radial slit for allowing the adaptor to deform reversibly sufficiently to fit snugly onto said container.

BRIEF DESCRIPTION OF THE DRAWING

The preferred embodiments of this invention, illustrating all its features, will now be discussed in detail. These embodiments depict the novel and non-obvious method and valve of this invention shown in the accompanying drawing, which is for illustrative purposes only. This drawing includes the following Figures, with like numerals indicating like parts:

FIG. 1 is a perspective view of the first embodiment of the valve of this invention.

FIG. 2 is an exploded perspective view of the valve shown in FIG. 1 illustrating the spike, seal, and the body or housing components of the invention.

FIG. 3 is a longitudinal cross-sectional view of the assembled valve of FIG. 1.

FIG. 4 is a schematic, longitudinal, cross-sectional view of the assembled valve of FIG. 1 before compressing the seal.

FIG. 5 is a schematic, longitudinal, cross-sectional view similar to FIG. 4 showing the valve during compression of the seal.

FIG. 6 is a perspective view of a second embodiment of the invention.

FIG. 7 is a longitudinal cross-sectional view of the valve of FIG. 6.

FIG. 8 is a schematic illustration of an ANSI delivery end of a medical implement compressing the seal of the valve of this invention.

FIG. 9 is a side elevation view, partially in cross-section, of a third embodiment of the seal.

FIG. 10 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using the seal of FIG. 9.

FIG. 11 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fourth embodiment of the seal.

FIG. 12 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fifth embodiment of the seal.

FIG. 13 is a longitudinal cross-sectional view of a sixth embodiment of the seal.

FIG. 14 is a longitudinal section of the seal shown in FIG. 13 used in connection with the spike device shown in FIG. 2.

FIG. 15 is a longitudinal partial cross-sectional view of a seventh embodiment of the seal of this invention.

6

FIG. 16 is a longitudinal cross-sectional view, after assembly, of the embodiment of the valve shown utilizing the seal of FIG. 15.

FIG. 17 is a longitudinal cross-sectional view, after assembly, of the eighth embodiment of the valve of this invention.

FIG. 18 is a longitudinal cross-sectional view, after assembly, of the ninth embodiment of the valve of this invention.

FIG. 19 is a side elevation view, after assembly, of the seal and spike shown in FIG. 14 connected to the body or housing shown in FIGS. 20 and 21.

FIG. 20 is a cross-sectional view taken along line 20—20 of FIG. 19.

FIG. 21 is a perspective view, with sections broken away to show the wall structure of the cavity containing the seal shown in FIGS. 13 and 14.

FIG. 22 is a greatly enlarged, cross-sectional view taken along line 22—22 of FIG. 14.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

The term “proximal” is used to denote the end of the valve and other components at or near the spike tip 32 in FIGS. 2 through 5, 10 through 12, 14, and 16, and at or near the spike tip 60 in FIG. 6, and at or near the seal cap 92 in FIGS. 8, 9, 13 through 19. The term “distal” is used to denote the opposite end of the valve, or spike tip, or seal. The term “medical implement” is used to denote any medical tool known to those of skill in the art that can connect to the present invention and facilitate the passage of fluids, particularly liquids, through the instant invention. Examples of medical implements that are contemplated include, but are not limited to, tubing, conduit, syringes, IV sets (both peripheral and central lines), piggyback lines, and other components which can be used in connection with a medical valve. Medical implements are commercially available in standard sizes. Thus, either or both ends of the valve of this invention can be provided with fittings to accommodate such standard size medical implements.

As best shown in FIGS. 1 and 2, the first embodiment of the invention, valve 10, includes a valve body or housing 12, a spike element 24, and a seal 36. The seal 36 is prepared from a resilient material that is flexible, inert, impermeable to fluid, and readily pierceable by the spike 26. In the embodiment shown in FIG. 13 depicting an alternate shaped seal 36d, this seal 36d has a precut slit 11 in its proximal end. This provides a tiny orifice through which the tip 32 of the spike element 24 may easily pass, yet still provides a fluid tight seal upon withdrawal of the spike element. These three components are assembled, as depicted in FIG. 3, with the spike element 24 enclosed to prevent accidental sticks. FIG. 2 illustrates how the housing 12, seal 36, and spike element 24 are attached without the need to use any adhesive or other bonding agent or process. Mechanical connection which provides a fluid tight closure is attained as is discussed subsequently. As shown in FIGS. 4 and 5, the seal 36 moves within the housing 12, being pierced by the spike element 24 to expose the tip 32 of the spike element 24 to allow fluid to flow through the valve 10.

Referring to FIG. 1, one preferred embodiment of housing 12 has a bell-shaped skirt 16 and an upper, preferably cylindrical, conduit 20. The skirt 16 is integral with, and connected by an annular ring 14, to the upper conduit 20. The skirt 16 creates a shield for an inner conduit 18 of the

5,928,204

7

spike element **24**. This inner conduit **18** is preferably cylindrical in shape, and slightly tapered. Inner conduit **18** and upper conduit **20** comprise aligned hollow tubes so that inner conduit **18** and upper conduit **20** are in fluid communication with one another when the spike element **24** pierces the seal **36**. There is an annular lip **25** surrounding a circular opening **25a** in the top of the conduit **20** (see FIG. 2).

In the first embodiment, the upper conduit **20** is adapted to receive the tip or nose **48** of an ANSI standard syringe **46** (see FIGS. 4 and 5). It is, however, contemplated that the outer diameter of the upper conduit **20** can be of any size to accommodate the attachment of other connector devices thereto. Advantageously, the proximal end of the upper conduit **20** can be equipped with a locking mechanism to facilitate locking of the valve **10** to a variety of connector devices. For example, referring to FIG. 1, locking ears **22** near the proximal lip **25** of housing **12** are preferably provided such that the housing **12** can be locked into any compatible Luer-Lock device known to those with skill in the art. For example, referring to FIG. 19, conventional Luer-Lock threads **180** can be provided on the outer diameter of upper conduit **20**.

Referring to FIG. 2, the spike element **24** has at its distal end the inner conduit **18** and at its proximal end a hollow spike **26** which is integral with the inner conduit. The inner conduit **18** and spike **26** present a continuous passageway for fluid during use. An annular cuff **28** on an intermediate portion of the spike element **24** is integral with, and interconnects, the inner conduit **18** and the spike **26**. As illustrated in FIG. 3, the rim **28a** of the cuff **28** abuts the underside of the inner ring **14**, and has an annular detent **28b** that snaps into an annular groove **14b** in the underside of the ring. The cuff **28** serves two functions. First, it serves as an attachment device to the underside of the annular ring **14**. Second, it serves as a support and attachment device for the seal **36**.

The hollow spike **26** has a tapered conical shape, ending in a sharp, pointed tip **32**. Preferably, along the length of the spike are raised, protruding ridges **30**. These raised ridges **30** extend from the surface of the spike preferably between 0.2–2.0 mm. The ridges **30** are preferably aligned along the length of the spike as illustrated in FIG. 2. These ridges **30** serve to break any vacuum created when the spike **26** is sealed as described hereinbelow. Modifications to the alignment and orientation of the ridges are discussed hereinbelow in association with their function. Just distal the spike tip **32**, there is situated at least one longitudinal through-hole **34** to permit fluid communication between the inner conduit **18** and the upper conduit **20**. Preferably, there are three through-holes **34** within about 0.200 inch from the spike tip **32**. These through-holes **34** may be of any size, however, the larger the size of the through-holes the greater the fluid flow rate through the valve **10**. In a preferred embodiment, the size of the through-holes **34** are 18-gauge to provide a flow rate three times that of a standard 18 gauge needle.

The seal **36** has a seal cap **40** with a generally flat top surface **40b**, an outwardly tapered sidewall **38**, and a lower lip **42**. Its interior is hollow to provide the conically shaped cavity **37** (FIG. 3). Thus, the seal **36** slips easily over the spike element **24** to fit snugly within the cavity **37**. The seal lip **42** is seated within the annular cuff **28** and wedged between the cuff and the underside of the ring **14**. There are longitudinal grooves **43** (FIG. 2) along the length of the seal **36** which provide air pockets that facilitate compression of the seal **36** during use. The grooves **43** may be of variable shape or size to facilitate seal-compression. In the first embodiment, there is a single groove **43** which completely surrounds the seal **36** between the seal cap **40** and the lip **42**.

8

The base of the seal **36** has a width such that the seal lip **42** fits snugly into the annular cuff **28**. The hollow interior or cavity **37** (FIG. 3) of the seal **36** is preferably tapered to conform internally to the shape of the spike **24**, having a wall portion **44** which contacts the spike **24** distal seal cap **40**. The exterior of the seal **36** is sized and shaped to fit inside the upper conduit **20** of the housing **12**. The cap **40** reseals the valve **10** when the top surface **40b** is above the through-holes **34**. Preferably, the cap **40** substantially fills the opening **25a** in the top of the conduit **20**. Thus, after assembly, the top surface **40b** of the seal cap **40** is essentially flush with the lip **25**, so that the lip **25** and seal cap **40** can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve **10**. It is important that the surface **40b** be exposed so that it may be swabbed with a disinfectant.

As best shown in FIG. 3, the spike **24**, with contiguous inner conduit **18**, is affixed to the housing **12** through the association of the external portion of annular cuff **28** and the internal portion of annular ring **14**. Although not necessarily required, these two pieces may be affixed by any one of a variety of methods known to those of skill in the art including, but not limited to, heat sealing, glue, pressure lock, bonding or the like. The seal **36** fits into the annular cuff **28** and is held in place by an internal lip **27** along the internal portion of the annular ring **14** of the housing **12**. The length of the spike **24** is such that, after assembly, the tip of the spike rests below the plane defined by the lip **25** of the housing **12**. Preferably, the spike tip **32** is approximately from 0.525" to 0.1" below the lip **25** of the housing **12**. The seal **36** fits snugly against the spike **24** and is essentially flush with the lip **25** of the housing **12**. The spike tip **32** is thus embedded within the seal cap **40** prior to use or may be approximately 0.025" distal the seal cap **40** when the valve **10** is in the closed position. The inner conduit **18** is partially shielded by the bell shaped skirt **16** of the housing **12** (see FIGS. 1–3). The inner surface of the bell shaped skirt **16** preferably has protruding threads **44** as an optional locking mechanism for attaching a medical implement thereto. Further, other medical devices can be pressure fit over the outer portion of inner conduit **18** without direct association with the protruding threads **44**.

During use, the invention is designed to be adapted as a two-way valve. The orientation of the valve is independent to fluid flow and dependent on the preferred orientation of the preexisting connections. Thus, the invention can be used as a valve connector for an intravenous central or peripheral piggyback connector in either orientation. Parenteral fluid is delivered to patients through tubing such that the liquid flows from a container through a needle into the patient. The containers are frequently changed or additional fluid bottles are added. The invention disclosed herein is designed to interconnect medical implements along the route of fluid delivery to the patient. However, the invention is also useful in any environment in which a resealable fluid valve is desired. During use, a connector of the appropriate size is fitted over the inner conduit **18**. Locking can be achieved by a Luer-Lock mechanism, a pressure fit or any other locking mechanisms known to those with skill in the art, as described above. Thus, in one example, fluid passes from the inner conduit **18** into the spike **26**. However, fluid flow is locked in place by the seal **36**.

FIGS. 4 and 5 illustrate valve activation. In FIG. 4, the medical implement connecting to the proximal end of the valve **10** is a syringe **46**. However, this connecting implement could be any number of medical implements known to those of skill in the art. The nose **48** of the syringe **46** is placed on the seal cap **40** inside the lip **25** of the housing **12**.

5,928,204

9

The application of pressure on the syringe **46** in the direction of the arrows, as illustrated in FIG. **4** creates pressure on seal cap **40**. The resulting downward pressure compresses the seal **36**. This pushes the tip **32** of the spike **26** through the seal cap **40** to expose the through-holes **34**. Compression is facilitated by the grooves **38**. Fluid is now able to flow into the syringe **46**, or vice versa, depending on whether fluid is to be withdrawn from the patient or medication injected into the patient. FIG. **5** shows valve **10** opened by insertion of the nose **48** of the syringe **46** into the opening **25a**. A syringe plunger **49** in the syringe **46** is retracted thereby creating a vacuum to draw fluid through the valve **10** into the syringe. For intravenous applications, the valve **10** can be orientated in the position diagramed in FIGS. **4** and **5**, or it can be rotated 180° such that fluid flows in the opposite direction.

Upon removal of the syringe from spike **26**, as shown in FIG. **4**, the seal **36** is free to return to its original shape and cover through-holes **34**. The ability of the seal **36** to return to its original shape is determined by the resiliency of the material used to prepare the seal **36**. In addition, the ability of the seal **36** to return to its original shape is facilitated by the protruding ridges **30** formed on the external surface of the spike. During compression, a vacuum may form in the area between the spike **26** and the seal **36**, thereby preventing the seal **36** from returning to its original position. The protruding ridges permit air to pass along the spike/seal interface to prevent vacuum formation and allow free return of the seal. The ability of the seal **36** to deform reversibly and return to its original position is particularly useful because (1) it immediately stops fluid flow through the valve **10**, (2) it covers the recessed spike **26** to maintain its sterility, and (3) it reduces the risk that the spike could inadvertently pierce another object or person. In addition, since the valve **10** lacks movable parts, except for the seal, it is unlikely that when the seal **36** is pushed down, the valve **10** would fail to function.

Advantageously, the through-holes **34** are located relatively low on the spike **26**. Thus, the through-holes **34** are sealed relatively early in the process as the seal **36** returns to its original configuration with the valve **10** is closed. In one preferred embodiment the through-holes **34** are located 0.075" below the spike tip **32** (see FIG. **2**). Additionally, the through-holes **34** are sealed even if the seal **36** does not fully return to its original configuration depicted in FIG. **4**. Further, the ability of the seal **36** to return reversibly to its original position permits the reuse of the connector valve **10**. Following disconnection, and before reuse, the surface of pierced seal cap **40** is essentially flush with the housing **12**. Thus, this flush surface can, advantageously be sterilized with alcohol or other surface decontaminating substances. The skirt **16** and upper conduit **20** advantageously shield both connections from the surrounding environment to protect the sterility of the connection. Further, both the skirt **16** and upper conduit **20** function as collection reservoirs to prevent fluid from dripping from the valve **10** during manipulation.

A cover cap (not shown) can be supplied to fit over the upper conduit **20** as further protection for the seal surface between use. Such a cover cap, however, is not needed to maintain sterility since the seal **36** may be swabbed with a disinfectant after each use. The reversibility of the seal **36** makes the valve **10** particularly attractive as a connector valve to provide fluid communication between two fluid lines. Therefore, the present invention provides for placing a first fluid line in communication with a second fluid line using the valve disclosed herein. The reversibility of the valve **10** permits multiple fluid lines to be successively

10

added, for example, to a fluid line in direct communication with a patient's vein. Since the valve is easily sterilizable and sealable, fluid lines can be added and removed without disconnecting venous contact.

The valve **10** is preferably prepared from a hard plastic, but it is additionally contemplated that the valve could be prepared from other medically inert materials known to those in the art. The spike element **24** is preferably prepared from the same material as the housing **12**. One particular advantage of this invention is that it does not rely on the use of metal needles. This dramatically reduces the risk of skin puncture during use and manufacture. Further, the upper conduit **20** serves as a shield to the spike **26** such that skin puncture is further reduced. The spike **26** need only be strong enough to penetrate the seal cap **40**, or if necessary, to pierce a connecting septum.

In the embodiment of the invention illustrated in FIGS. **2-4**, the through-holes **34** are placed distal spike tip **32**. This placement provides two important advantages. First, the placement of the through-holes **34** facilitates resealing of the valve **10** after use. Second, if the through-holes were placed at the spike tip **32**, the holes **34** may core the seal cap **40** thereby introducing seal particulate into the fluid flow and possibly plugging the holes **34**. Thus, the longitudinal placement of the through-holes distal spike tip **32** prevents the introduction of particulates into the fluid path and/or plugging of the through-holes **34**. It is additionally contemplated that the number and diameter of the through-holes **34** can be adjusted to accommodate different fluid velocities. In a preferred embodiment, the preferred velocity of fluid passing through the through-holes **34** is equal to or greater than the flow rate through an 18 gauge needle. Through-holes larger than 18 gauge will, of course, facilitate greater fluid velocities.

An important advantage of the invention is that the valve **10** has very little dead space, thus the volume of liquid entering into the valve is substantially equivalent to the volume of fluid leaving the valve. Further, the total equivalent fluid volume of the valve is very small such that the volume of fluid flowing through the system in order to place the valve in fluid communication with a medical implement such as a syringe **46** is substantially zero.

Alternate Embodiments

In another preferred embodiment of the invention, illustrated by FIGS. **6** and **7**, a disposable sterile adaptor valve **50** is provided to function as a resealable lid for a container (not shown) of fluid. The fluid can thus be removed from the fluid container or permitted to flow from the container into a medical implement adapted to house fluid in a sterile manner. As is the conventional practice, an open mouth of the container will ordinarily be sealed with a cover member (not shown).

FIG. **6** shows an adaptor valve **50** having a body including an adaptor skirt **52**.

The adaptor skirt **52** will preferably fit snugly over the open mouth of the container. The skirt **52** may be of any size to accommodate a range of container sizes. A lengthwise slit **54** is preferably provided in at least one location along the length of the skirt to ensure a snug fit between the skirt **52** and the container. A chamber **56**, preferably tubular in configuration, extends upward from the skirt **52** and is similar in construction and design to the upper chamber **20** of the first preferred embodiment. Similar to the first embodiment, the proximal portion of the valve contains a locking mechanism **59** that preferably comprises a Luer-Lock device or other locking device known to those of skill in the art.

5,928,204

11

As depicted in FIG. 7 a spike 58 extends upward through a tubular chamber 56. A spike tip 60 is preferably recessed from a proximal lip 62 of the tubular chamber 56. In a closed position, this tip 60 is covered by a seal 64, which is essentially the same as seal 36. Protruding ridges 66 and seal grooves 68 facilitate seal compression in the open position and promote closure following use. Thus, in the closed position as illustrated in FIG. 7, the seal 64 covers the through-holes 70 to prevent fluid out-flow from the container. The adaptor valve 50 contains a second spike 72 which points in the opposite direction as spike 58. These spikes 52 and 72 are in fluid communication with each other. The spike 72 extends downward inside the adapter skirt 52. The two spikes preferably form one component of the valve 50 while the skirt 52 and upper chamber form a second component. These two components can be assembled in a manner like that of the valve 10. The spike 72, like the spike 58, has longitudinal through-holes 74 and a tip 76. The through-holes 74 are located inward of the tip 76. The adaptor valve 50 is thus useable with containers holding sterile medicament having a cover or septum seal at the open mouth of the container. Examples of containers with such seals contemplated for use with this invention include dosage bottles for intramuscular injector antibiotic containers or the like. However, it is also contemplated that the valve 50 can be adapted with its own seal and locking mechanism to permit the valve to be employed on a variety of containers for medicaments or other fluids. Medicaments in these types of containers are preferably maintained under sterile conditions and the volume and nature of the medicament is such that multiple aliquots are intermittently removed over time. If the medicament is reconstituted, then, during use, any covering over the opening on the container is removed to reveal the rubber septum. The adaptor valve 50 is placed over the septum and direct pressure is applied to pierce distal spike 72 through the septum and into the container. A syringe or the like can then be applied, as depicted in FIG. 4, in association with the first preferred embodiment, to withdraw fluid from the container. The pressure of the nose 48 over the spike 58 pushes spike tip 60 through seal 64. At the same time, seal 64 is pushed back and compresses. Compression is accommodated by seal grooves 68. Fluid is withdrawn from the container and the syringe is removed from the spike 58. Release of the pressure applied to seal 64 permits the seal to return to its original configuration. The spike ridges 66 facilitate seal reversibility.

Often the ingredients housed in containers are those that can be lyophilized at purchase. Lyophilized ingredients require reconstitution before use. If the medicament requires reconstitution before use, then sterile water, saline, or other fluid can be introduced into the container before fluid is extracted. The two-way nature of the valve permits this without any special adaptation. After the syringe is removed, the adaptor valve 50 automatically seals. Subsequently, aliquots can be removed from the container by syringe or the like. Alcohol or other compatible surface sterilizing agent can be used to wipe the lip 62 and seal 64 before each use. Similar to the first embodiment, it is additionally contemplated that a cap can be provided to fit over upper chamber lip 62 between use.

The adaptor valve 50 can be adapted to function as a medicament adaptor for an intravenous container. In this case, the adaptor valve 50 is placed on a medicament container for intravenous delivery and attached via tubing to an intravenous feed. Thus, the adaptor valve 50 can be placed in fluid communication with a connector valve of FIG. 1 to facilitate the flow of medicament from intravenous drip bottles.

12

An alternative embodiment of the seal, a seal 36a, is shown in FIG. 9. Seal 36a comprises a seal cap 92 at the proximal end thereof and a seal lip 96 at the distal end thereof. A cup-like annular flange 95 is provided proximal seal cap 92. The seal cap 92 and seal lip 96 are connected by a seal wall consisting of a plurality of ringed wall portions 94 that expand and collapse in an accordion like fashion. During compression of the seal 36a, the diameter of the ringed wall portions 94 expand outward in the radial direction. There are air pockets 13a (FIG. 10) between ring portions 94 and the housing and air pockets 13b between spike 24 and seal 36a. The seal 36a contains a cavity 98 distal seal cap 92 and adjacent the ringed wall portions 94. The seal 36a interacts with spike 26 (FIG. 2) and other components of the present invention in a similar fashion to seal 36 of FIG. 2.

Referring to FIG. 10, the cup-like annular flange 95 may be stretched around the upper conduit 20 and held in place by an annular ring 97. This creates a trampoline like effect that assists returning the seal 36a to a decompressed state after withdrawal of a syringe (not shown). This embodiment has two advantages. First, the proximal end of the valve 10 can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve 10. Second, by affixing cup-like annular flange 95 to upper conduit 20 at the proximal end thereof with annular ring 97, the repeated deformation and reformation of the seal 36a is assisted.

An alternative embodiment of the seal, a seal 36b is shown in connection with the valve 10 in FIG. 11. S The seal 36b is similar to the seal 36a and is comprised of seal cap 92, a side wall consisting of ringed wall portions 94 and a seal lip 96. It also has an outwardly extending ring 99 which is at a right angle with respect to the longitudinal axis of the valve 10. This ring 99 is used to attach the seal 36b to upper conduit 20. Preferably, an upper conduit annular plug 20' is inserted within upper conduit 20 to create a tight fit between perpendicular ring 99, a ledge 101 in the upper conduit 20, and the plug 20'. The ring 99 assists in the reformation of seal 36b to enclose spike 26 upon withdrawal of a syringe (not shown).

As shown in FIG. 12, the cup-like annular flange 95 and ring 99 may both be used in connection with the valve 10, to provide the seal 36c. This seal 36c, provides rapid reformation upon withdrawal of a syringe (not shown) and realizes the advantages of both the seals 36a and 36b.

Another alternative embodiment of the seal, a seal 36d, is shown in FIG. 13. In this embodiment, the seal 36d is comprised of seal cap 92, seal lip 96, and a side wall 150 comprised of circular tires 100 stacked in series on top of an adjacent larger diameter lower tire. The circular tires 100 are preferably solid throughout the diameter of the cross-section thereof. These circular tires 100 will deform and reform upon, respectively, compression and decompression of the seal 36d, thereby exposing or covering a spike (not shown) as the case may be.

As mentioned above, preferably seal 36d has a precut slit 11 in the cap 92 lying along the longitudinal axis of the valve 10. The seal cap 92 has a unique configuration that insures that the slit 11 closes and is sealed upon withdrawal of a syringe (not shown) and reformation of the seal 36d. It includes an enlarged, internal, pressure responsive member 200 which is integral with the cap 92. Between the proximal end of the side wall 150 and the member 200 is an annular space 102 which is filled with the fluid in the cavity 98. This fluid is under pressure, for example at the blood pressure of the patient to which the valve 10 is attached. Referring to

5,928,204

13

FIG. 14, fluid, for example the patient's blood, flows through the holes 34 in the spike 26, filling the cavity 102. This fluid presses against the exterior of the member 200, closing the slit 11 when the seal is decompressed as shown in FIGS. 14 and 19. The pressure from this fluid creates a high pressure seal which prevents fluid from escaping valve 10 through the slit 11. There is a semi-cylindrical annular flange tear ring 104 on the end of the member 200 which advantageously extends the useful life of seal 36d.

Preferably, there is a tear ring 104 integral with the member 200 along the perimeter of the internal surface the member 200, and a slight saucer-like depression 204 in the external surface of the seal. The pressure responsive element in the decompressed state closes any orifice in the seal 36d to provide an essentially-fluid-tight seal while in the decompressed state. The pressure responsive member 200 enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve 10 is connected to a patient's artery. The center of the member 200 and the annular space 102 are coaxial with the entryway 11a to the orifice 11. The pressurized fluid fills the annular space 102 to apply pressure that compresses the member 200 to tightly close the entryway to the orifice. In a preferred embodiment the distance from the entryway 11a to the proximal end of seal cap 92 is from 0.500 to 0.075 inches and more preferably approximately 0.100 inch.

As best illustrated in FIG. 22, the tip 32 is designed to avoid tearing the seal. Tip 32 has three facets 210, 212, and 214 which are joined with each other along parting lines a, b, and c. This junction of the facets 210, 212, and 214 frequently is ragged and will tear the seal 36d. This is prevented by the parting lines a, b, and c, or junctions, being disposed within recesses 220, 222, and 224, respectively, to provide "buried parting lines."

Another alternative embodiment of the present invention using the seal 36d is shown in FIG. 8 and FIGS. 19 through 21. In this embodiment, the inner wall 160 of the upper end of the conduit 20 is provided with at least one, and preferably, a plurality of radial indentations 107. The indentations 107 are elongated disposed generally parallel to the longitudinal axis of the valve 10 in a symmetrical, star-like configuration. Each indentation has opposed lateral edges 162 which engage the seal 36d upon compression of the seal 36d. The indentations provide space into which the seal 36d expands upon compression.

As best shown in FIG. 8, the wall 181 of the proximal end of the conduit 20 is tapered inward at the same angle as the nose 48 of the syringe 46. In accordance with ANSI standards, the taper is 0.006 inch per linear inch. The wall 182 of the syringe nose 48 bears against the wall 181 as the nose slides into the opening 25a to push the seal 36d inward compressing it and forcing the tip 32 of the spike 36 to enter the slit 11. The seal 36d expands upon compression to fill essentially completely the upper portions of the indentations 107. Some sections of the seal 36d are wedged between the edges 162 and other sections fill the indentations 107. As the liquid flows through the nose 48 through holes 34, air in the nose 48 is forced out of the nose 48 and expelled from valve 10 between walls 181 and 182. Thus, essentially the entire prescribed dosage is delivered through valve 10 to the patient. Fluid flows through the through-holes 34, but does not leak between either the seal 36d and the wall 181 or between the abutting walls 181 and 182.

FIGS. 15, 16, 17, and 18 depict embodiments of seals, namely, seal 36e, seal 36f, and seal 36g, which are substan-

14

tially the same as the seals 36a (FIG. 10), seal 36b (FIG. 11), and seal 36c (FIG. 12), except the side wall 150 employing the circular tires 100 is used in place of the accordion wall portion 94.

Other components of the present invention interact with the various embodiments of the seal in a similar fashion to their interaction with seal 36 of FIG. 2. Prior to use of valve 10, it is preferable that the seal caps 40 or 92 be pierced centrally by a steel needle in the axial direction, precutting the seal to provide the slit 11 in order to allow for more rapid decompression and reformation of the seal upon piercing by the spike 26. The seals are advantageously formed from a material which can repeatedly reseal and prevent fluid from flowing around the seal material. The seal 36 should also be capable of being forced down and then spring back into position to reseal the valve. Material that is too soft will reseal effectively; however, will not be capable of springing back after opening of the valve. Material that is too hard will provide sufficient spring force; however, will not effectively seal. Thus, in a preferred embodiment, the seal is formed from a silicone having a hardness in the range from 30-70 Shore durometer units, and more preferably in the range 40-50 Shore durometer units. A cure silicone polymer in the preferred hardness range is available from Wacker Silicone Corp. of Adrian, Mich. In some embodiments of the invention, it is desirable to provide additional lubricity to the seal 36 to allow it to spring back and reseal more effectively. Dow Chemical Co. produces a silicone formulation with silicone oil built in to provide this additional lubricity.

In general, the closing of the valve 10 is provided not by the side wall of the seal 36 which immediately covers the through-holes 34, but by the seal cap 40, or seal cap 92 filling the proximal end of the cavity 98 and the opening 25a. Thus, the seal caps 40 and 92 are sufficiently thick to reseal the opening 25a effectively after valve closure. However, the seal caps 40 and 92 should also be sufficiently thin to allow them to readily return to the closed position. Preferably the thickness of the caps 40 and 92 ranges between 0.075 and 0.500 inch and more preferably may be approximately 0.100 inch.

The valve disclosed in this invention can be provided in a sterile and disposable form such that after its use in a given installation is exhausted, the device is discarded. However, as described above, in any given installation, the device can be reused multiple times. Since the device does not employ needles, there is little chance that the device will inadvertently cause skin puncture. Therefore, the extra precautions required for handling and disposing of needles is obviated. It will be apparent from the detailed description provided herein that the present invention can provide for the elimination of nearly all needles used in the medical environment. With the use of the valve of the present invention, the need for all needles except those that are directly input into a patient is, advantageously, eliminated.

Operation

The valve 10 is used to provide a closed, patient access system for transferring a predetermined amount of medication from a remote source to the patient. The valve 10 is connected by the distal end to the patient, for example, a vein or artery in fluid communication with the valve. Blood fills the valve, but the seal 36d, for example, prevents any blood from leaking from the valve. The delivery end or nose 48 of the medical implement is inserted into the valve as depicted in FIG. 8, pushing the nose 48 against the seal to compress the seal sufficiently to allow the tip 32 of the spike

5,928,204

15

24 to pierce the seal and enter said delivery end. The predetermined amount of medication in its entirety may now be transferred through the nose 48 into the valve 10 and into the patient. Since the nose 48 and seal 36d engage in a manner so that the tip 32 of the spike element 24, upon piercing the seal, meets the seal to avoid formation of any dead space at the interface between nose 48 and the seal surface 40b. Transfer directly through the valve 10 of essentially the entire predetermined amount of medication from the syringe 46 to the patient, so that essentially none of said predetermined amount is collected in any dead space in the valve, is accomplished with this invention. Upon withdrawing the nose 48 from the valve 10 the seal 36d returns to the decompressed state to close the valve and maintain while in said decompressed state a fluid tight seal even at high pressures and after repeated uses.

Scope of the Invention

The above presents a description of the best mode contemplated of carrying out the present invention, and of the manner and process of making and using it, in such full, clear, concise, and exact terms as to enable any person skilled in the art to which it pertains to make and use this invention. This invention is, however, susceptible to modifications and alternate constructions from that discussed above which are fully equivalent. Consequently, it is not the intention to limit this invention to the particular embodiments disclosed. On the contrary, the intention is to cover all modifications and alternate constructions coming within the spirit and scope of the invention as generally expressed by the following claims, which particularly point out and distinctly claim the subject matter of the invention.

I claim:

1. A seal for use in selectively opening and closing a fluid pathway through a medical connector comprising a resilient seal element having a wall having a top end and a bottom end, said wall including at least two generally arcuate segments each having an outwardly extending portion, said segments intersecting one another and defining at least one space between where said segments intersect and a line tangential to the outwardly extending portions of both segments, and at least one segment proximate to said bottom end having a larger maximum diameter than a second segment nearer to said top end of said element.

2. The seal element in accordance with claim 1, wherein said seal element has a centerline therethrough and a generally hollow interior, and wherein said outwardly extending portions of said arcuate segments extend in a direction perpendicular to said centerline.

3. The seal element in accordance with claim 1 wherein said seal element has a centerline therethrough and wherein said outwardly extending portions of said arcuate segments extend in a direction away from said centerline.

4. The seal element in accordance with claim 1, wherein said arcuate segments are defined by ring-elements, each ring element having a generally "c"-shaped cross-section with a top end and a bottom end and a central portion, said rings joined at their top and bottom ends, and said central portion defining said outwardly extending portions.

5. The seal element in accordance with claim 1, wherein said arcuate segments are defined by stacked ring elements, said ring elements having a generally circular cross-section and said outwardly extending portion comprising an outer surface of said ring element.

6. An element for use in selectively opening and closing a fluid flow path through a medical device, comprising:
a generally cylindrical member having a wall with a first end and a second end, said wall forming at said first end

16

a unitary resealable opening, said member having an inner surface and an outer surface and a centerline extending between said ends, at least one of said surfaces having alternating radially inwardly and radially outwardly extending surfaces with respect to said centerline, said wall comprising a generally resilient material in at least the area of said alternating surfaces and said wall having at least two ring-shaped elements, each element having a diameter and an exterior surface and defining a central passage therethrough, said ring-shaped elements being joined to each other such that their central passages are aligned along said centerline, the diameter of each successive ring-shaped element increasing in a direction from said first end to said second end, and at least some portion of said alternating surfaces being defined by said exterior surfaces of said joined ring-shaped elements, whereby the application of a compressive force along said centerline decreases the length of said member, and when said force is removed, said member generally returns to its original length.

7. The element in accordance with claim 6, wherein said ring-shaped elements have a circular cross-section.

8. The element in accordance with claim 6, wherein at least one ring element has a "c"-shaped cross-section, said cross section having a top end, a bottom end, and a central portion, said ring element being joined to an adjacent ring element at said top end and another adjacent ring at said bottom end, and said central portion defining said exterior surface of said ring element.

9. A seal element for use in selectively opening and closing a fluid pathway through a medical connector comprising a resilient, generally conical seal element having a first end and a second end and a wall, said wall defining an inner surface and an outer surface of said element, said wall forming at said first end a resealable opening, said element having a centerline extending through said first and second ends thereof, and wherein the radial distance of at least one of said outer or inner surfaces from said centerline alternately varies from a first distance from said centerline to a second distance from said centerline which is different than said first distance moving in a direction from said first end to said second end.

10. The element in accordance with claim 9, wherein at least some portion of said element is comprised of a series of O-ring elements stacked together and connected to form a unitary structure.

11. A seal element for use in selectively opening and closing a fluid pathway through a medical connector comprising a resilient, generally frusto-conical seal element having a first end and a second end and a wall, said wall defining an inner surface and an outer surface of said element, said wall forming at said first end a resealable opening, said element having a centerline extending through said first and second ends thereof, and wherein the radial distance of at least one of said outer or inner surfaces from said centerline alternately varies from a first distance from said centerline to a second distance from said centerline which is different than said first distance moving in a direction from said first end to said second end.

12. The element in accordance with claim 11, wherein at least some portion of said element is comprised of a series of O-ring elements stacked together and connected to form a unitary structure.

* * * * *

EXHIBIT D



US006572592B1

(12) **United States Patent**
Lopez

(10) **Patent No.:** US 6,572,592 B1
(45) **Date of Patent:** *Jun. 3, 2003

(54) MEDICAL VALVE AND METHOD OF USE

(75) Inventor: **George A. Lopez**, Corona del Mar, CA
(US)

(73) Assignee: **ICU Medical, Inc., San Clemente, CA**
(US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: 09/569,712

(22) Filed: **May 9, 2000**

3,172,205 A	3/1965	Gammon
3,354,881 A	11/1967	Bloch
3,416,567 A	12/1968	Von Dardel et al.
5,549,577 A	8/1996	Siegel et al.
5,556,388 A	9/1996	Johlin, Jr.

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

BG	61386	1/1992
CN	1077654 A	10/1993
EP	0 240 987	4/1987
NO	310805	6/1994
RU	2 154 462	8/2000
WO	WO 86/01712	3/1986
WO	WO 86/03415	6/1986
WO	WO 86/03416	6/1986
WO	WO 91/06255	5/1991
WO	WO 93/11828	6/1993

* cited by examiner

Primary Examiner—Brian L. Casler

Assistant Examiner—LoAn H. Thanh

(74) *Attorney, Agent, or Firm*—Knobbe, Martens, Olson & Bear LLP

(57) **ABSTRACT**

(63) Continuation of application No. 08/905,370, filed on Aug. 4, 1997, now abandoned, which is a continuation of application No. 08/334,846, filed on Nov. 4, 1994, now Pat. No. 5,685,866, which is a continuation of application No. 08/096,659, filed on Jul. 23, 1993, now Pat. No. 5,695,466, which is a continuation-in-part of application No. PCT/US92/10367, filed on Dec. 1, 1992, now abandoned, which is a continuation-in-part of application No. 07/813,073, filed on Dec. 18, 1991, now abandoned.

(51) **Int. Cl.**⁷ **A61M 5/14**
(52) **U.S. Cl.** **604/256; 604/905**
(58) **Field of Search** 604/244, 246,
604/249, 256, 905; 137/844, 845, 859


(56) **References Cited**

U.S. PATENT DOCUMENTS

1,578,517 A	3/1926	Hein
2,289,677 A	7/1942	Perelson
2,342,215 A	2/1944	Perelson
2,387,512 A	10/1945	Hilberg
2,667,986 A	2/1954	Perelson
2,847,995 A	8/1958	Adams
3,134,380 A	5/1964	Armao
3,135,261 A	6/1964	Carroll

A closed system, needleless valve device includes a generally tubular body defining an internal cavity. On the proximal end of the body there is an opening which is preferably sufficiently large to receive an ANSI standard tip of a medical implement. The distal end of the body has a generally tubular skirt. The valve also includes a hollow spike having a closed tip. The spike includes at least one longitudinal 18-gauge hole located distal the tip, and is seated inside the cavity such that the tip is below the proximal end of the body. An annular support cuff is connected to the spike which seals off a portion of the cavity of the body such that an upper cavity containing the tip is defined. The valve also includes a plastic, resilient silicone seal which fills the upper cavity and opening and covers the tip of the spike so as to present a flush surface. An adaptor enables the valve to be attached to a resealable container.

46 Claims, 19 Drawing Sheets

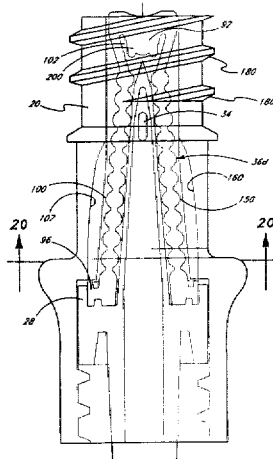


US 6,572,592 B1

Page 2

U.S. PATENT DOCUMENTS

3,648,684 A	3/1972	Barnwell et al.	4,850,978 A	7/1989	Dudar et al.
3,788,519 A	1/1974	Mengal	4,874,377 A	10/1989	Newgard et al.
3,813,791 A	6/1974	Stewart et al.	4,875,291 A	10/1989	Panique et al.
3,852,385 A	12/1974	Huggins	4,875,760 A	10/1989	Youngren et al.
3,974,832 A	8/1976	Kruck	4,878,897 A	11/1989	Katzin
3,976,063 A	8/1976	Henneman et al.	4,880,414 A	11/1989	Whipple
3,976,073 A	8/1976	Quick et al.	4,889,527 A	12/1989	Herrli
3,986,508 A	10/1976	Barrington	4,891,469 A	1/1990	Whitehouse et al.
3,993,063 A	11/1976	Larrabee	4,898,452 A	2/1990	Kawachi et al.
4,019,512 A	4/1977	Tenczar	4,900,310 A	2/1990	Ogle, II
4,059,112 A	11/1977	Tischlinger	4,907,879 A	3/1990	Webb
4,076,285 A	2/1978	Martinez	4,915,687 A	4/1990	Sivert
4,079,738 A	3/1978	Dunn et al.	4,917,668 A	4/1990	Haindl
4,080,965 A	3/1978	Phillips	4,928,212 A	5/1990	Benavides
4,121,585 A	10/1978	Becker, Jr.	4,943,896 A	7/1990	Johnson
4,128,098 A	12/1978	Bloom et al.	4,950,260 A	8/1990	Bonaldo
4,133,314 A	1/1979	Bloom et al.	4,969,883 A	11/1990	Gilbert et al.
4,161,949 A	7/1979	Thanawalla	4,970,794 A	11/1990	Buckley
4,187,846 A	2/1980	Lolachi et al.	4,979,941 A	12/1990	Ogle, II
4,191,225 A	3/1980	Ogle	4,998,713 A	3/1991	Vaillancourt
4,201,208 A	5/1980	Cambio, Jr.	4,998,921 A	3/1991	Vickory et al.
4,214,779 A	7/1980	Losell	4,998,927 A	3/1991	Vaillancourt
4,219,912 A	9/1980	Adams	5,009,490 A	4/1991	Kuono et al.
4,294,249 A	10/1981	Sheehan et al.	5,018,532 A	5/1991	Ethridge, III
4,296,949 A	10/1981	Muettterties et al.	5,024,616 A	6/1991	Ogle, II
4,306,705 A	12/1981	Svensson	5,033,476 A	7/1991	Kasai
4,311,382 A	1/1982	Buckley et al.	5,046,456 A	9/1991	Heyman et al.
4,328,802 A	5/1982	Curley et al.	D321,250 S	10/1991	Jepson et al.
4,329,987 A	5/1982	Rogers et al.	D321,251 S	10/1991	Jepson et al.
4,334,551 A	6/1982	Pfister	D321,252 S	10/1991	Jepson et al.
4,338,933 A	7/1982	Bayard et al.	5,064,416 A	11/1991	Newgard
4,343,550 A	8/1982	Buckley et al.	5,065,783 A	11/1991	Ogle, II
4,362,156 A	12/1982	Feller, Jr. et al.	5,069,225 A	12/1991	Okamura
4,392,499 A	7/1983	Towse	5,100,394 A	3/1992	Dudar et al.
4,411,662 A	10/1983	Pearson	5,122,123 A	6/1992	Vaillancourt
4,417,890 A	11/1983	Dennehey et al.	5,134,489 A	7/1992	Sauer
4,432,759 A	2/1984	Gross et al.	5,134,703 A	7/1992	Bonaldo
4,432,765 A	2/1984	Oscarsson	5,135,489 A	8/1992	Jepson et al.
4,439,188 A	3/1984	Dennehey et al.	5,154,703 A	10/1992	Bonaldo
4,439,193 A	3/1984	Larkin	5,158,554 A	10/1992	Jepson et al.
4,457,749 A	7/1984	Bellotti et al.	5,163,230 A	11/1992	Gast
4,461,091 A	7/1984	Gammon	5,163,922 A	11/1992	McElveen, Jr. et al.
4,470,664 A	9/1984	Shirasawa	5,167,642 A	12/1992	Fowles
4,508,367 A	4/1985	Oreopoulos et al.	5,167,647 A	12/1992	Wijkamp et al.
4,511,359 A	4/1985	Vaillancourt	5,167,648 A	12/1992	Jepson et al.
4,512,766 A	4/1985	Vaillancourt	5,171,234 A	12/1992	Jepson et al.
4,535,820 A	8/1985	Raines	5,188,620 A	2/1993	Jepson et al.
4,564,054 A	1/1986	Gustavsson	5,199,947 A	4/1993	Lopez
4,592,356 A	6/1986	Gutierrez	5,203,775 A	4/1993	Frank et al.
4,607,868 A	8/1986	Harvey et al.	5,211,638 A	5/1993	Dudar et al.
4,610,469 A *	9/1986	Wolff-Mooij	5,242,432 A	9/1993	DeFrank
4,614,437 A	9/1986	Buehler	5,251,873 A	10/1993	Atkinson et al.
4,617,012 A	10/1986	Vaillancourt	5,255,441 A	10/1993	Burgess et al.
4,623,068 A	11/1986	Brown et al.	5,256,155 A	10/1993	Yerlikaya et al.
4,624,667 A	11/1986	Ktnarak	5,269,771 A	12/1993	Thomas et al.
4,639,019 A	1/1987	Mittleman	5,273,533 A	12/1993	Bonaldo
4,645,494 A	2/1987	Lee et al.	5,290,254 A	3/1994	Vaillancourt
4,666,429 A	5/1987	Stone	5,295,657 A	3/1994	Atkinson
4,673,400 A	6/1987	Martin	5,323,539 A	6/1994	O'Neil
4,706,487 A	11/1987	Bandou et al.	5,344,414 A	9/1994	Lopez et al.
4,725,267 A	2/1988	Vaillancourt	5,380,306 A	1/1995	Brinon
4,735,607 A	4/1988	Keith, Jr.	5,385,547 A	1/1995	Wong et al.
4,752,292 A	6/1988	Lopez et al.	5,401,245 A	3/1995	Haining
4,759,756 A	7/1988	Forman et al.	5,411,499 A	5/1995	Dudar et al.
4,775,369 A	10/1988	Schwartz	5,423,753 A	6/1995	Fowles et al.
4,781,702 A	11/1988	Herrli	5,470,319 A	11/1995	Mayer
4,782,841 A	11/1988	Lopez	5,487,731 A	1/1996	Denton
4,784,650 A	11/1988	Coburn	5,509,912 A	4/1996	Vaillancourt et al.
4,810,241 A	3/1989	Rogers	5,549,566 A	8/1996	Elias et al.
4,826,500 A	5/1989	Rautsola	5,694,686 A	12/1997	Lopez
4,832,214 A	5/1989	Schrader et al.	5,695,466 A	12/1997	Lopez et al.
4,834,664 A	5/1989	Lin	5,700,248 A	12/1997	Lopez
4,846,809 A	7/1989	Sims	5,738,663 A *	4/1998	Lopez 604/249
			6,113,068 A *	9/2000	Ryan 251/149.4

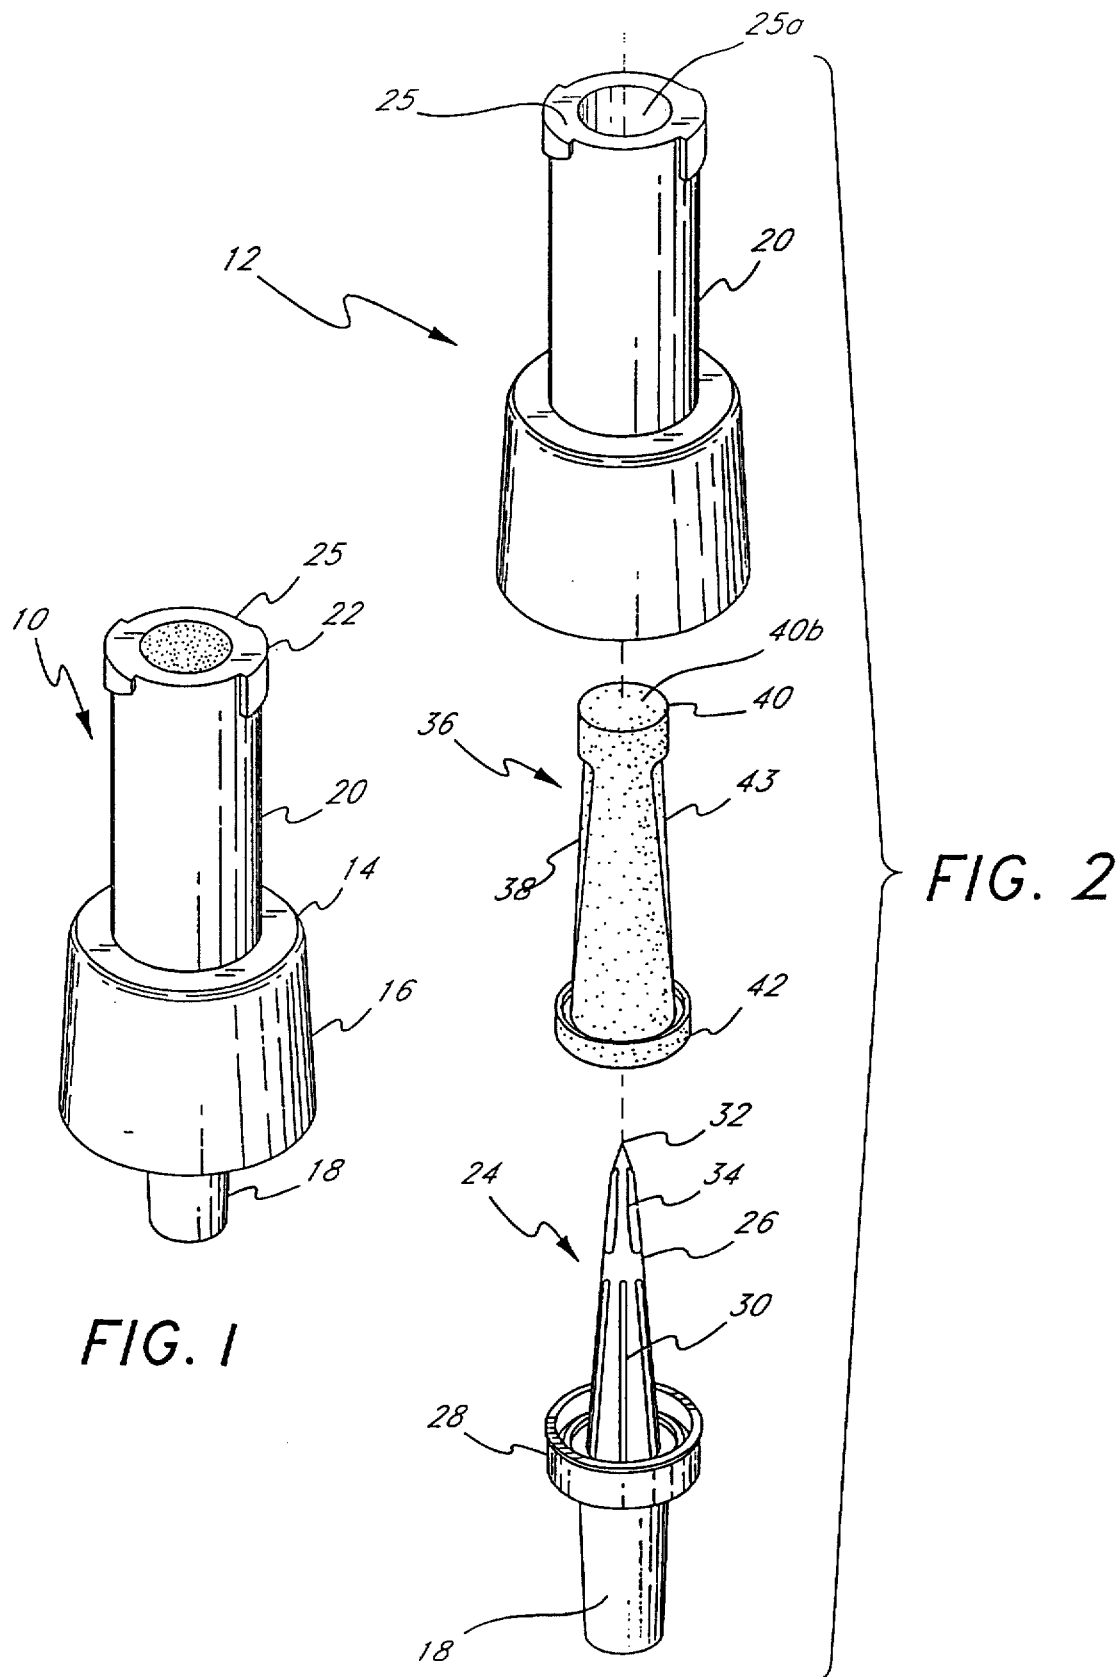

U.S. Patent

Jun. 3, 2003

Sheet 2 of 19

US 6,572,592 B1

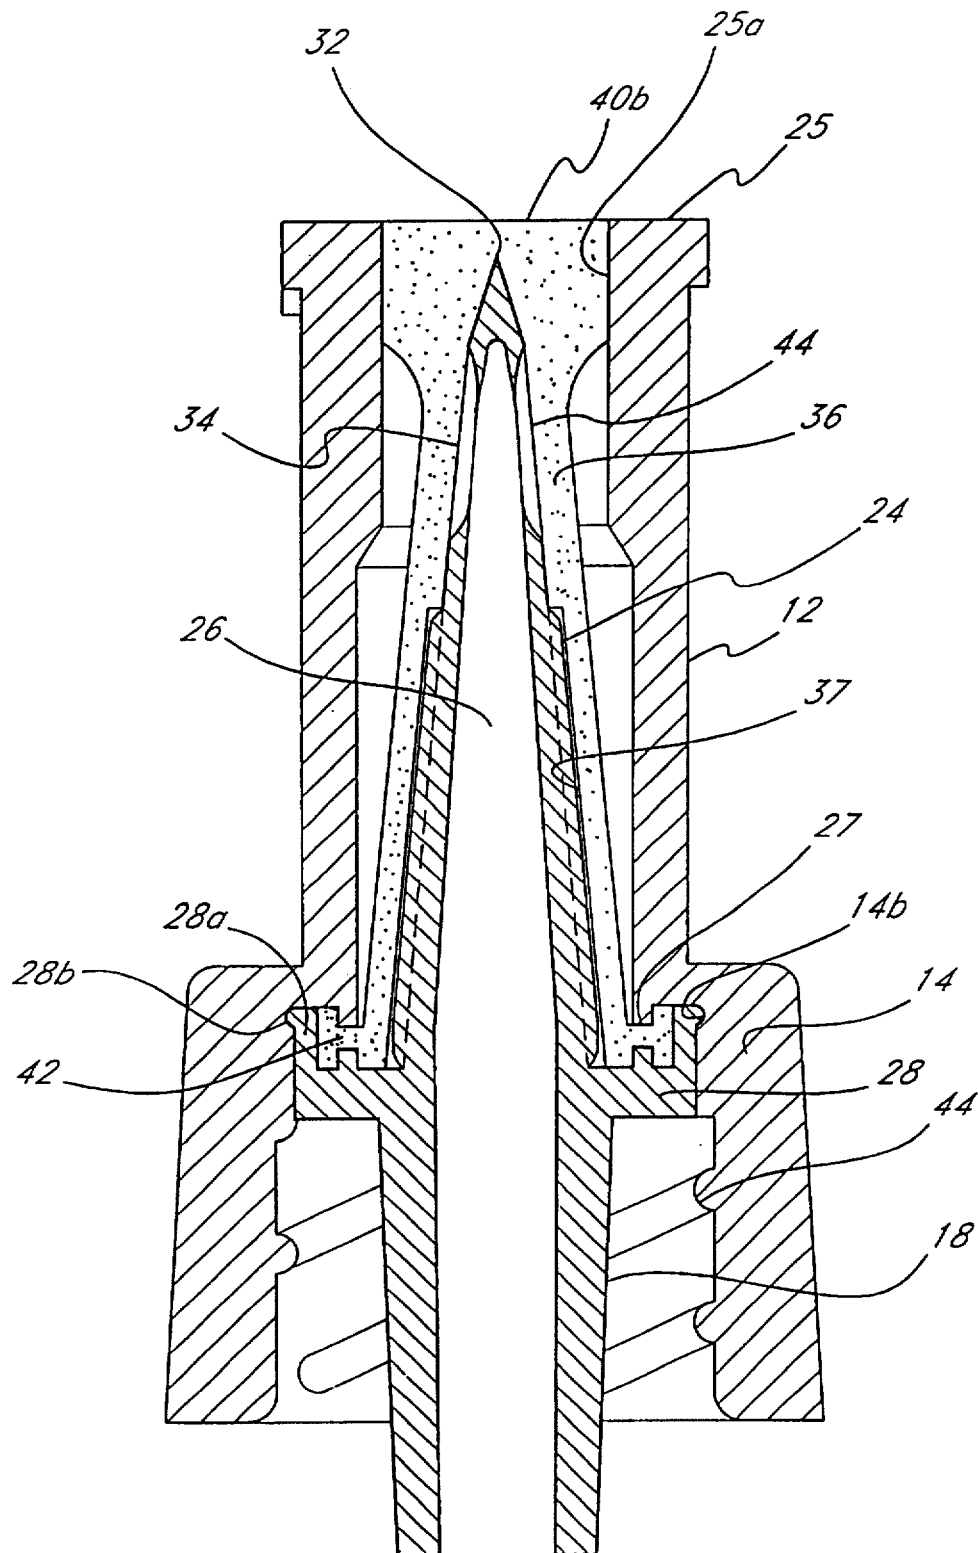


FIG. 3

U.S. Patent

Jun. 3, 2003

Sheet 3 of 19

US 6,572,592 B1

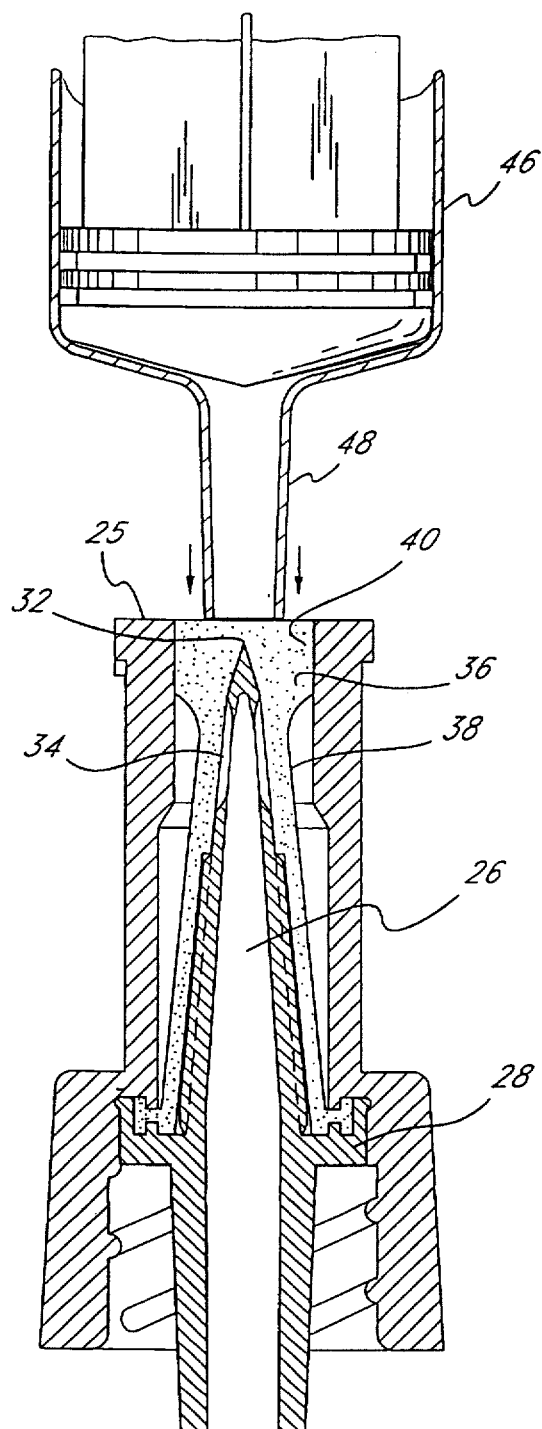


FIG. 4

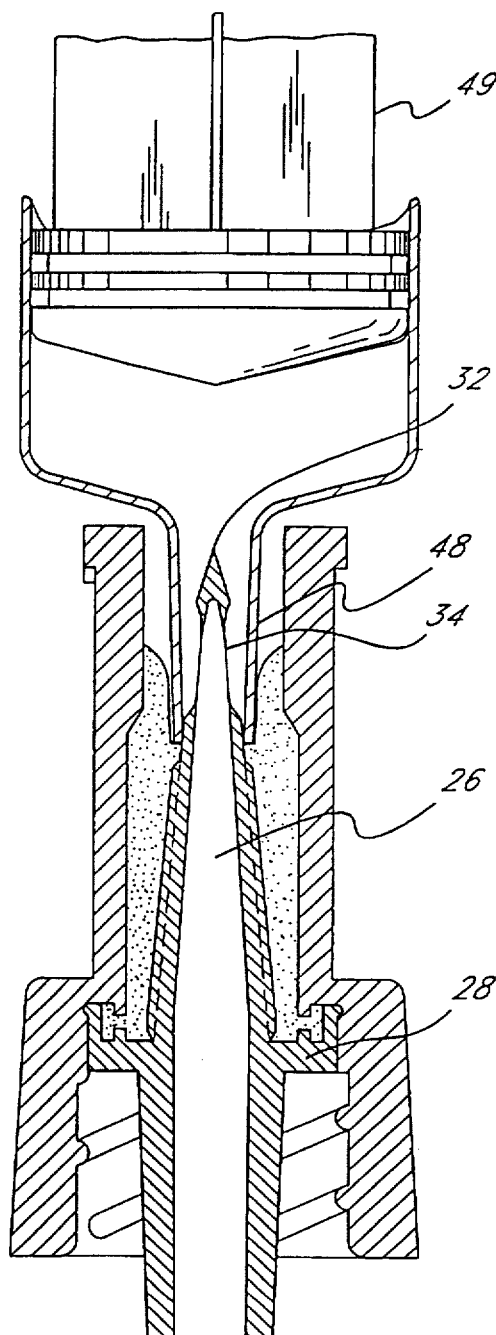


FIG. 5

U.S. Patent

Jun. 3, 2003

Sheet 4 of 19

US 6,572,592 B1

FIG. 6

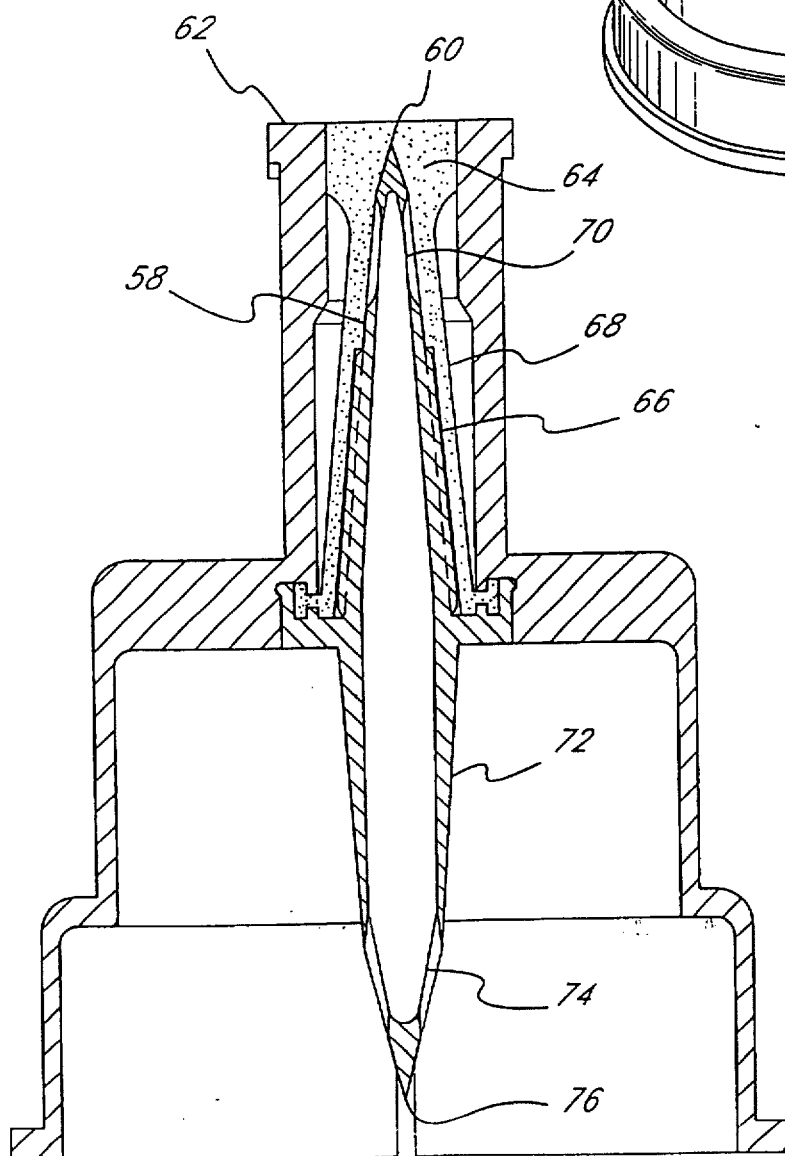
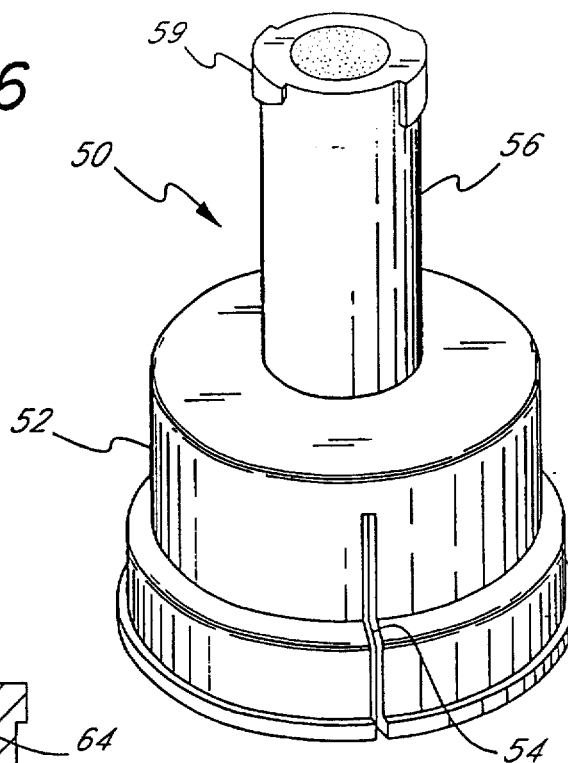


FIG. 7


U.S. Patent

Jun. 3, 2003

Sheet 5 of 19

US 6,572,592 B1

FIG. 8

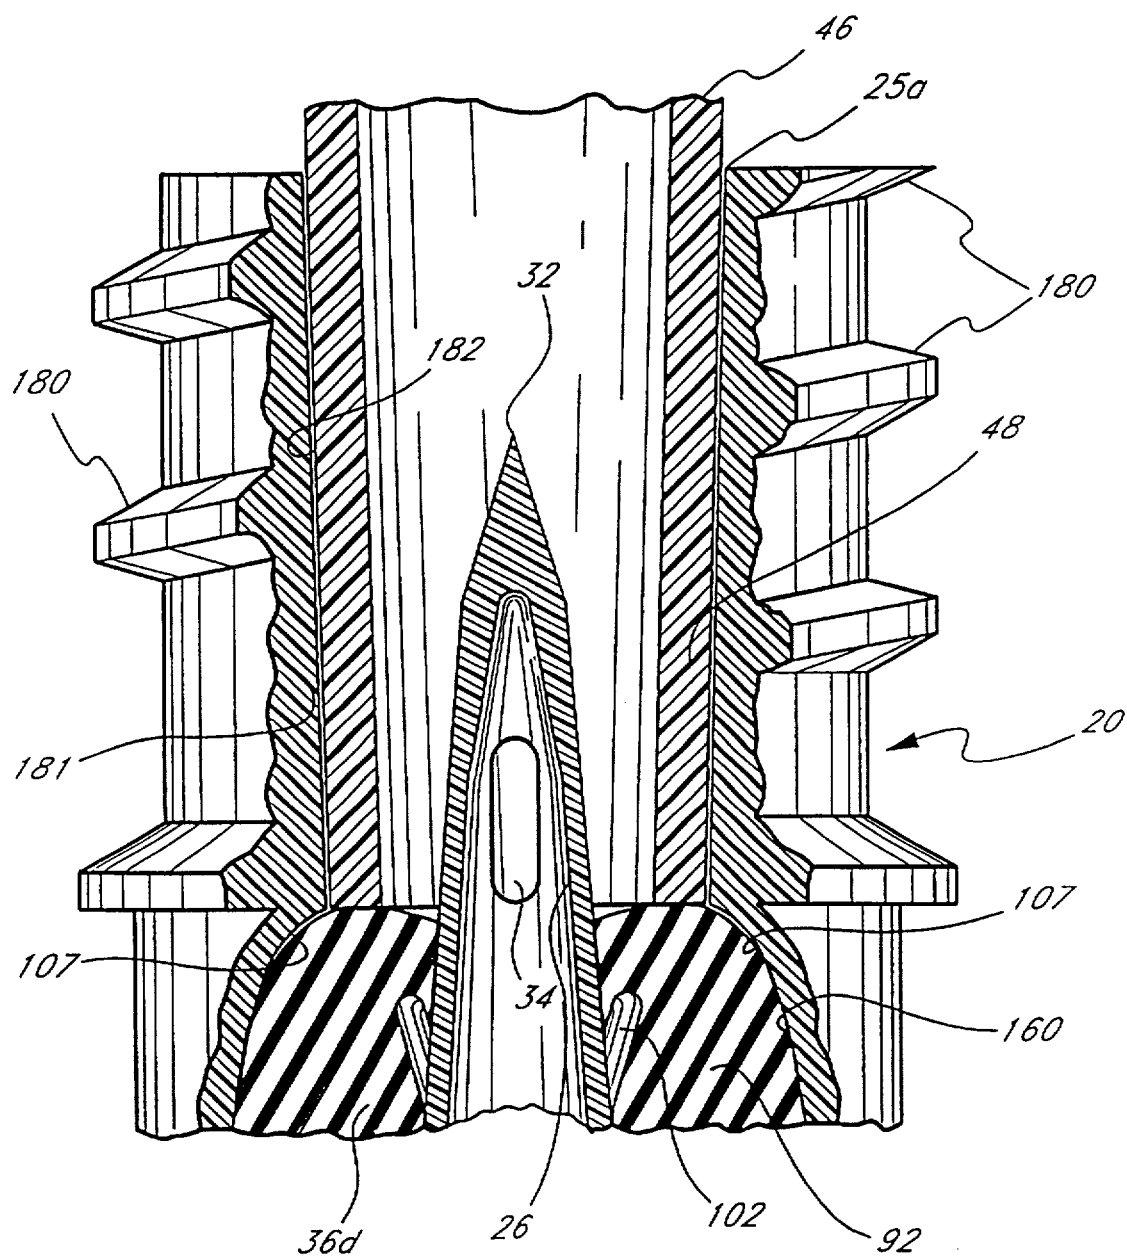

U.S. Patent

Jun. 3, 2003

Sheet 6 of 19

US 6,572,592 B1

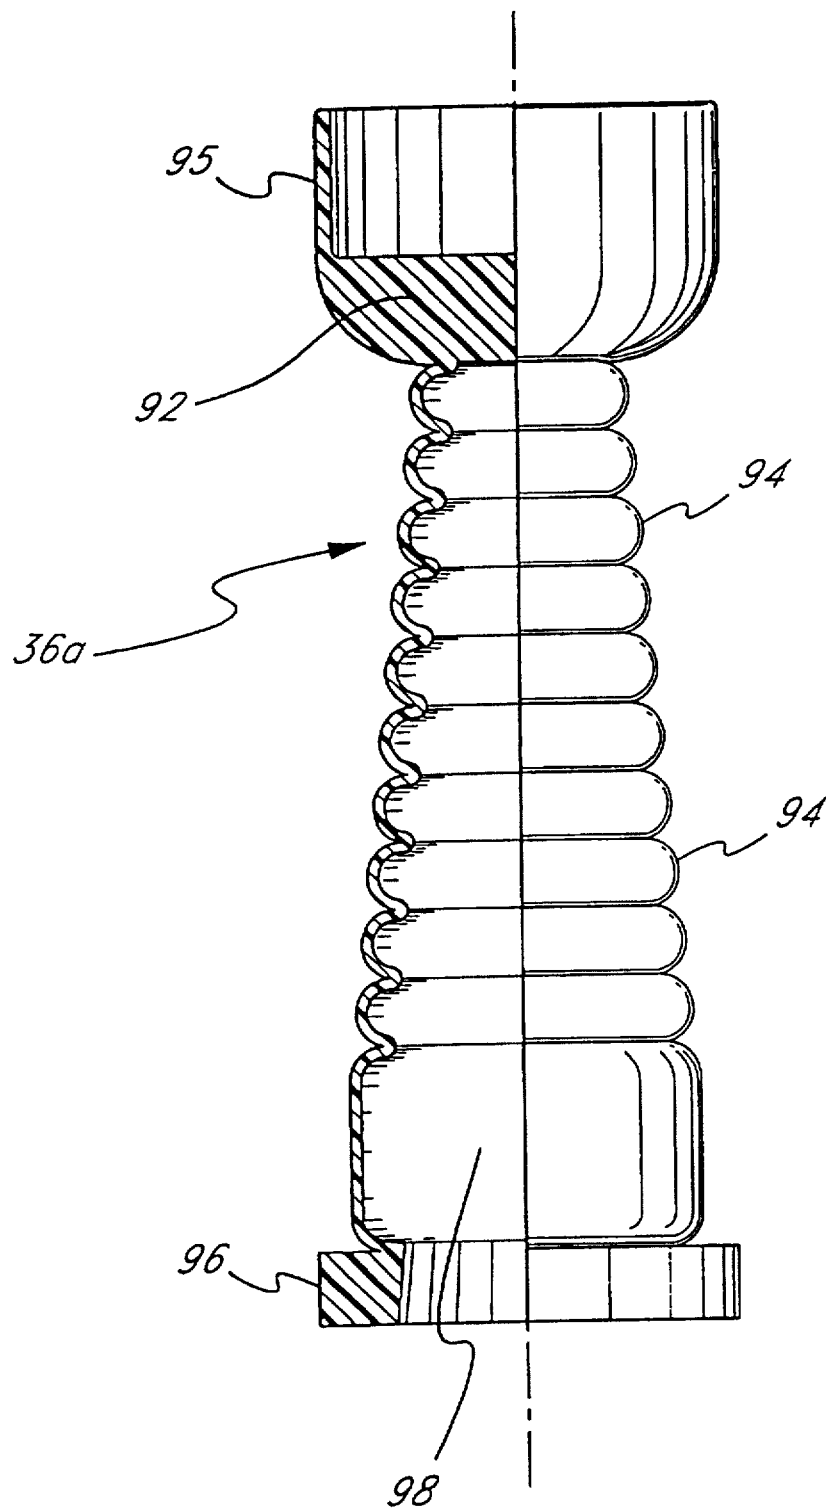


FIG. 9

U.S. Patent

Jun. 3, 2003

Sheet 7 of 19

US 6,572,592 B1

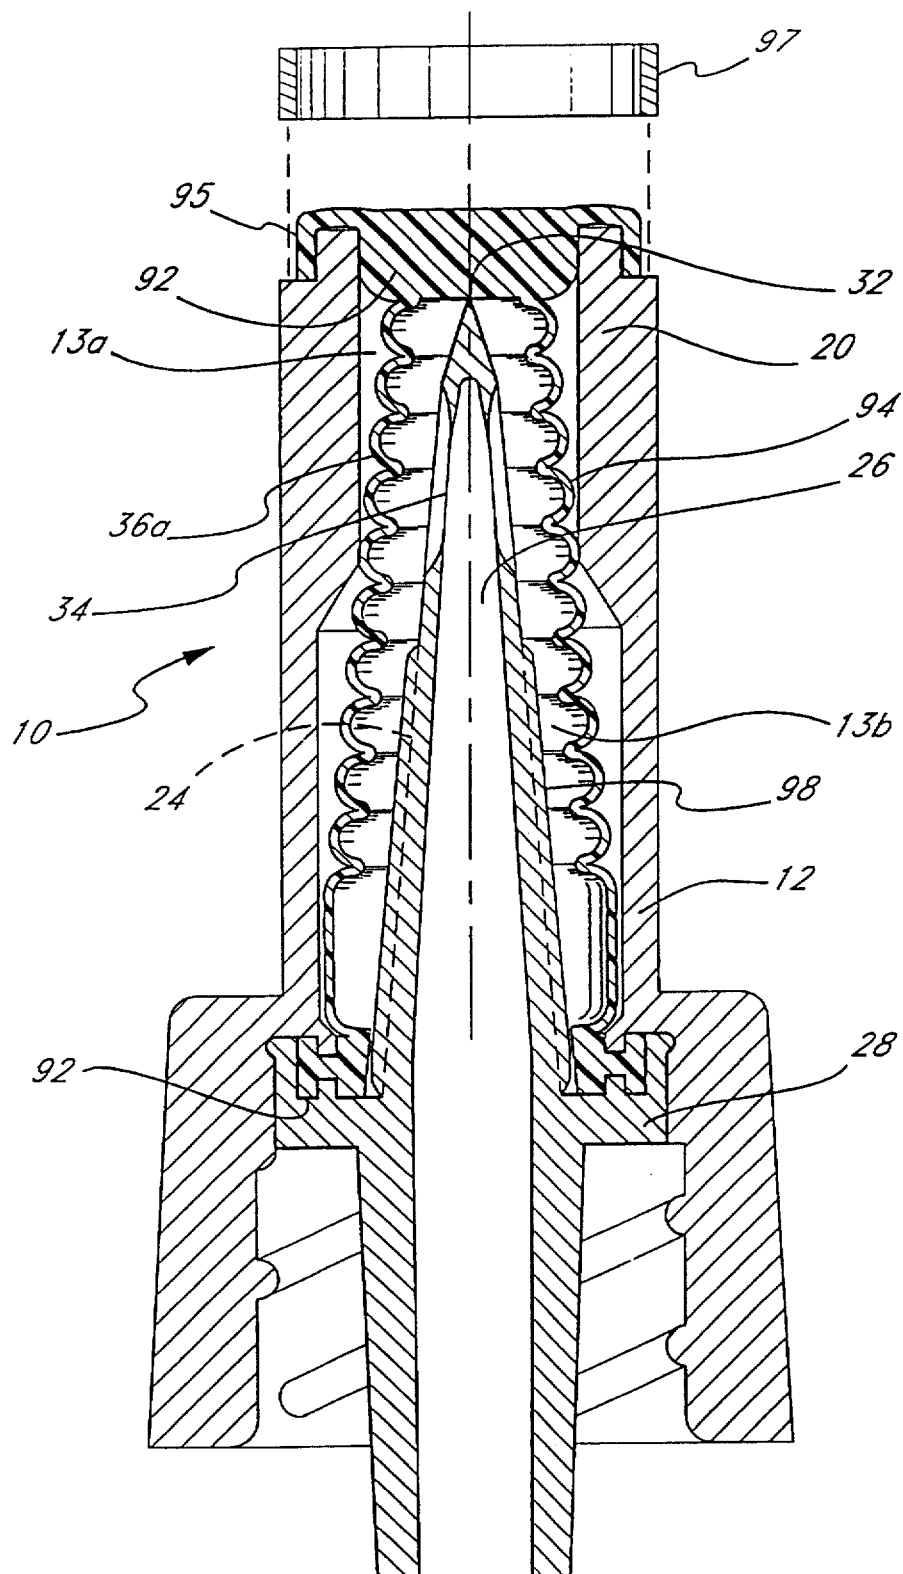


FIG. 10

U.S. Patent

Jun. 3, 2003

Sheet 8 of 19

US 6,572,592 B1

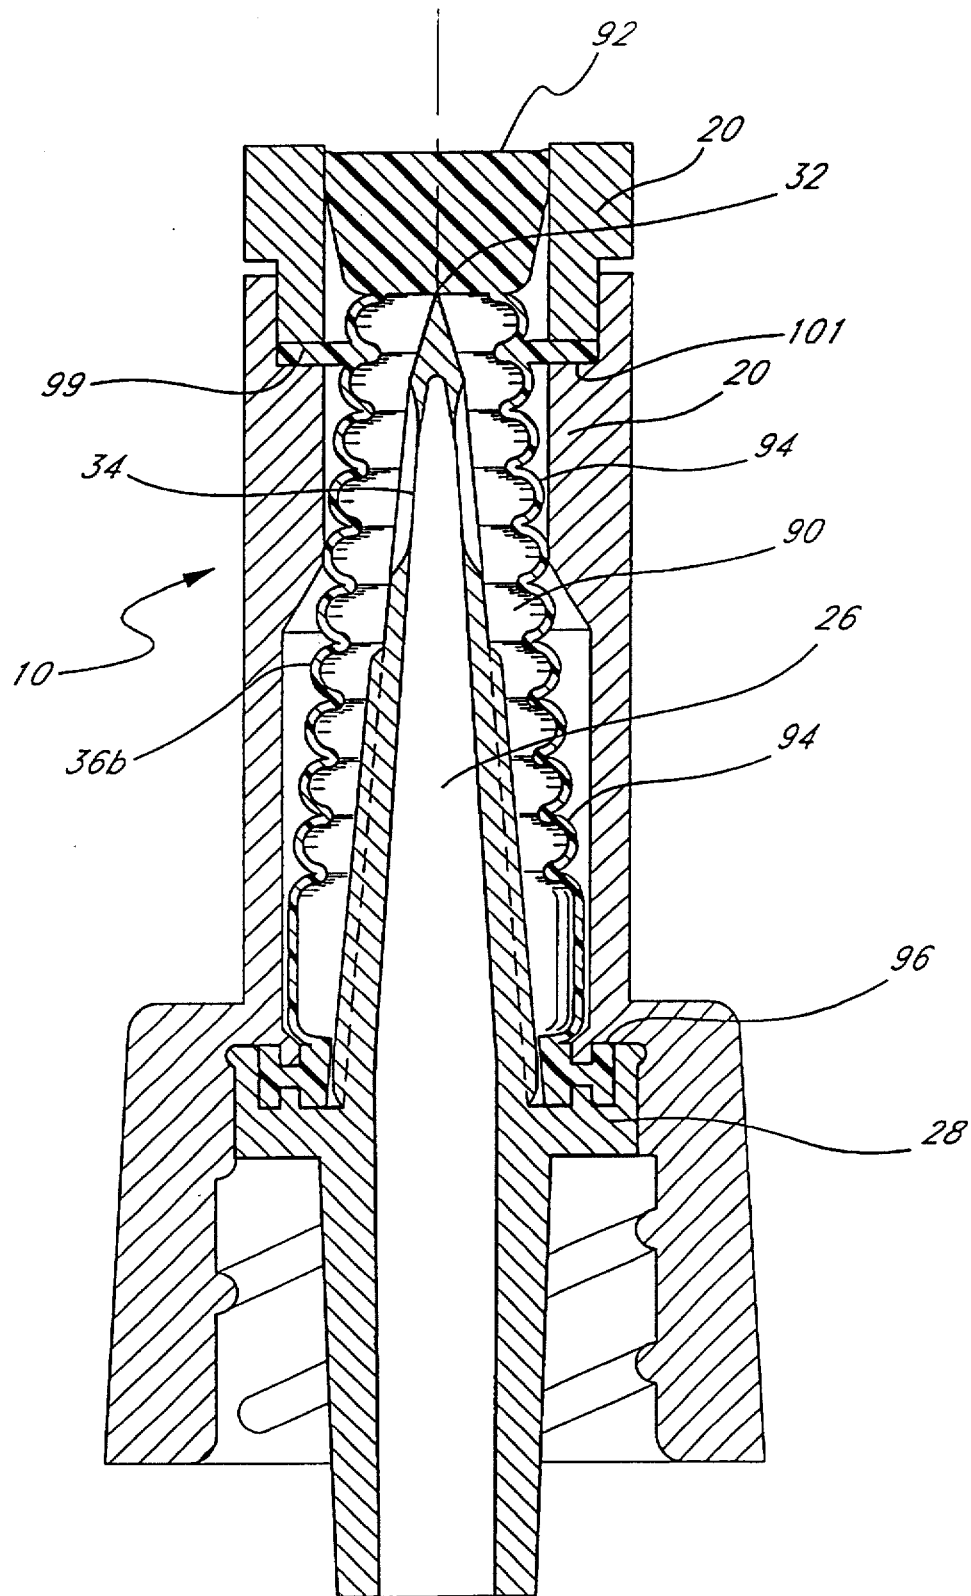


FIG. 11

U.S. Patent

Jun. 3, 2003

Sheet 10 of 19

US 6,572,592 B1

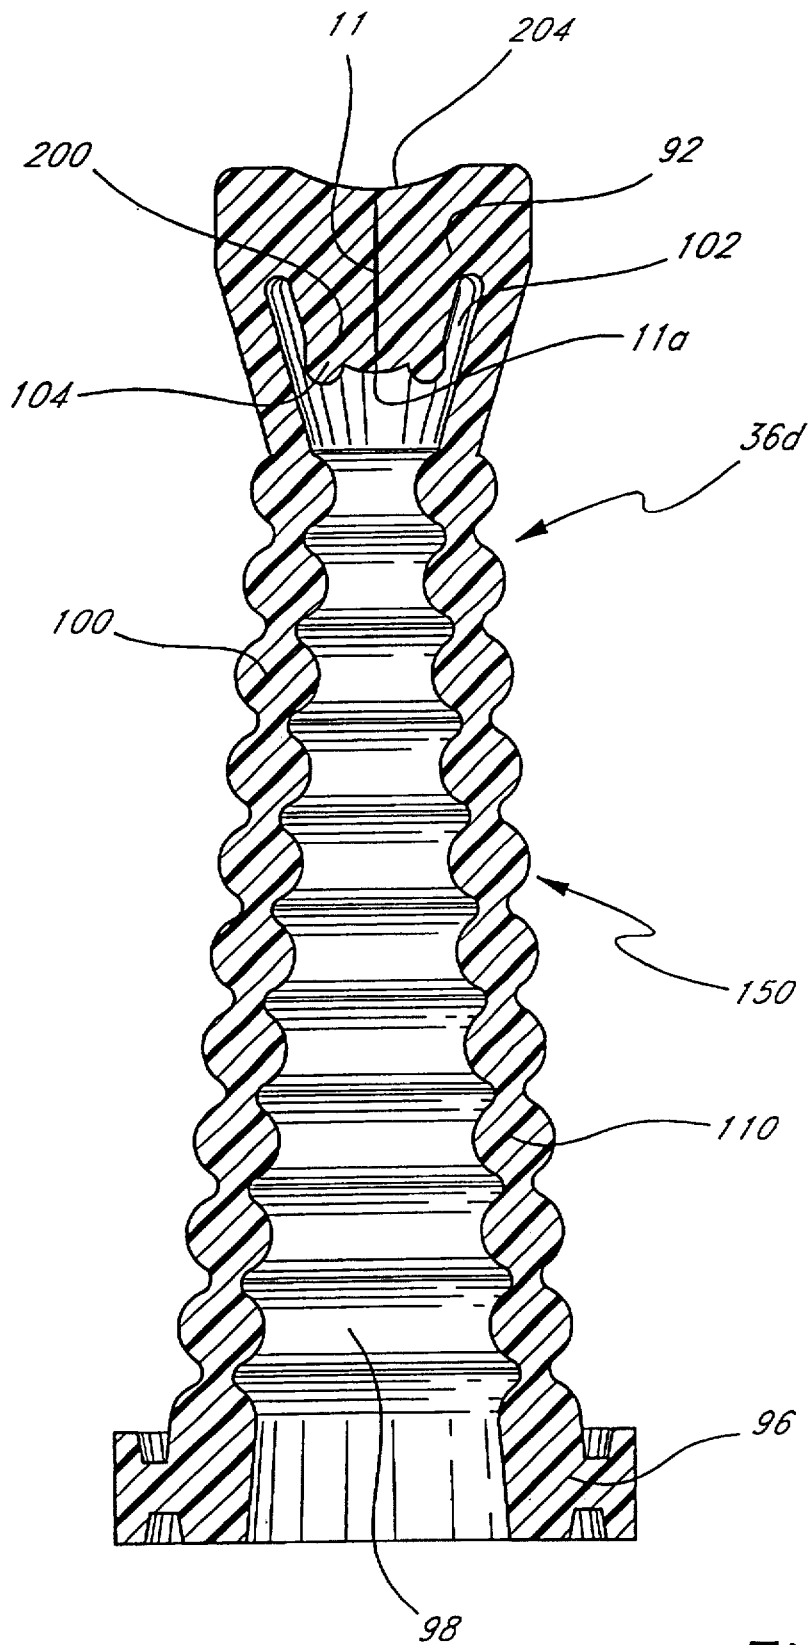


FIG. 13

U.S. Patent

Jun. 3, 2003

Sheet 11 of 19

US 6,572,592 B1

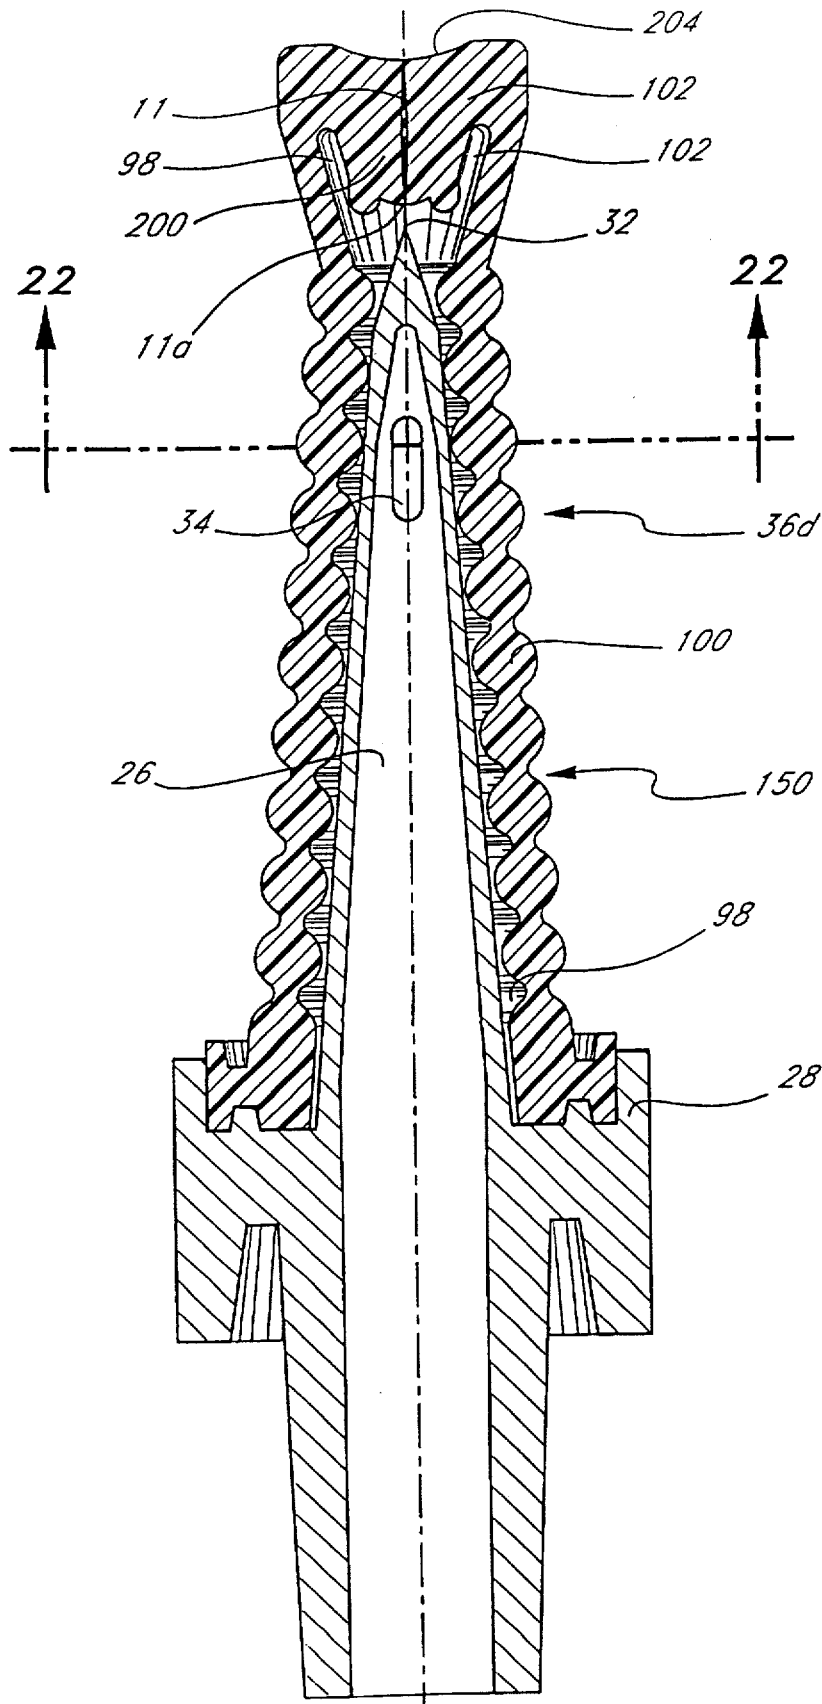



FIG. 14

U.S. Patent

Jun. 3, 2003

Sheet 12 of 19

US 6,572,592 B1

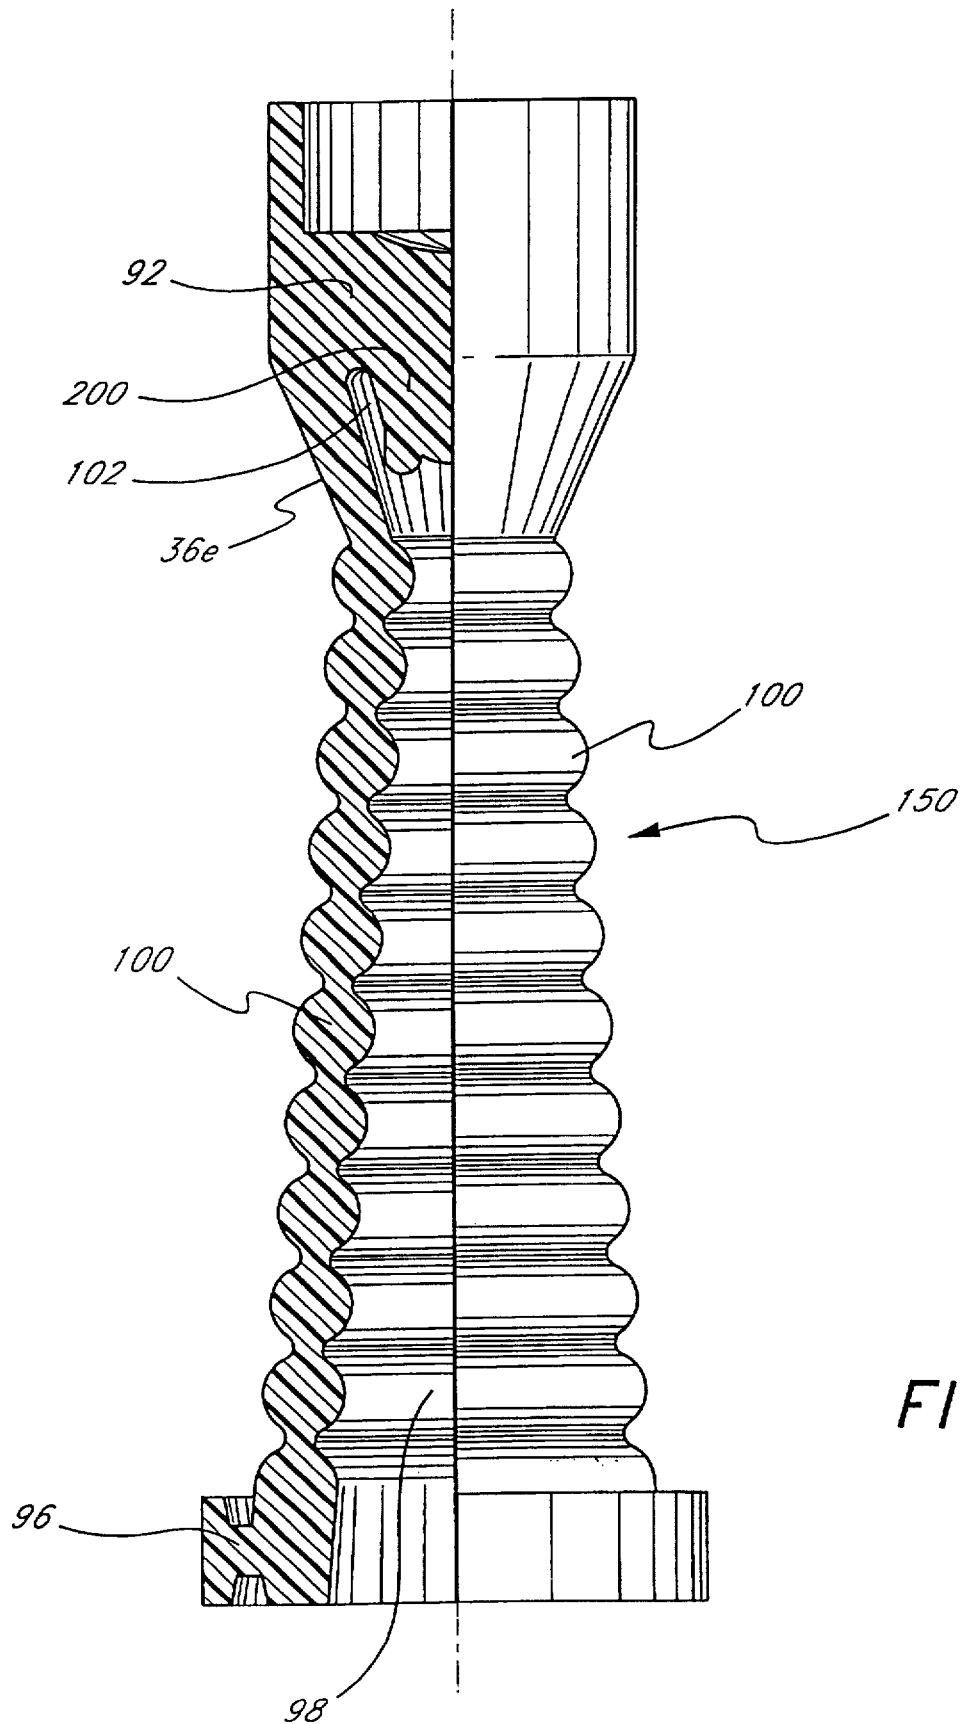

U.S. Patent

Jun. 3, 2003

Sheet 13 of 19

US 6,572,592 B1

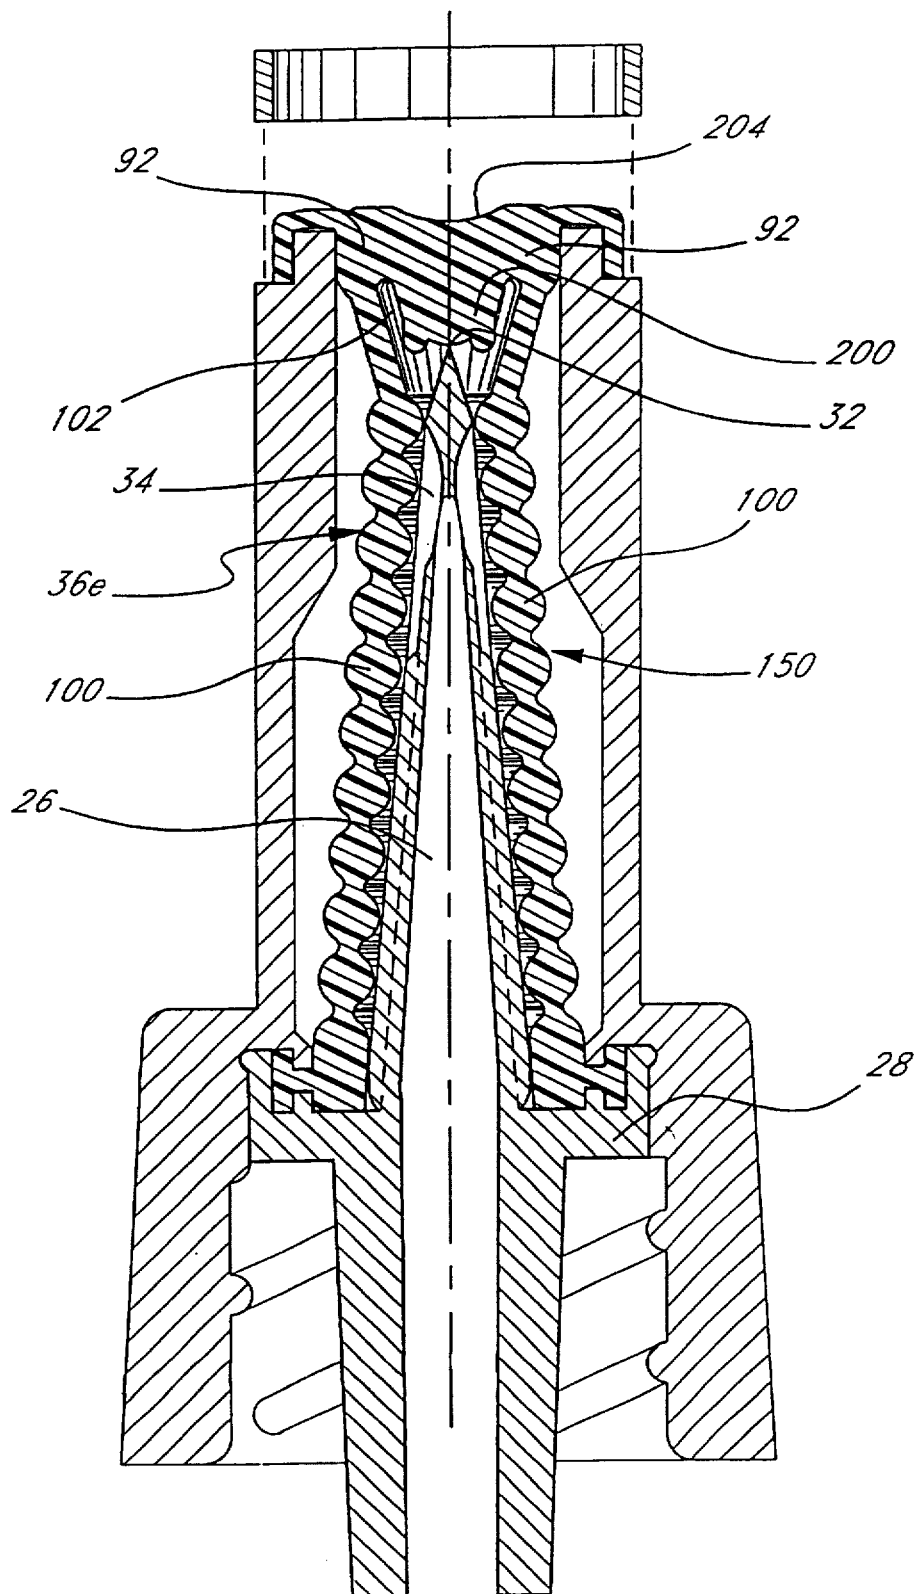


FIG. 16

U.S. Patent

Jun. 3, 2003

Sheet 14 of 19

US 6,572,592 B1

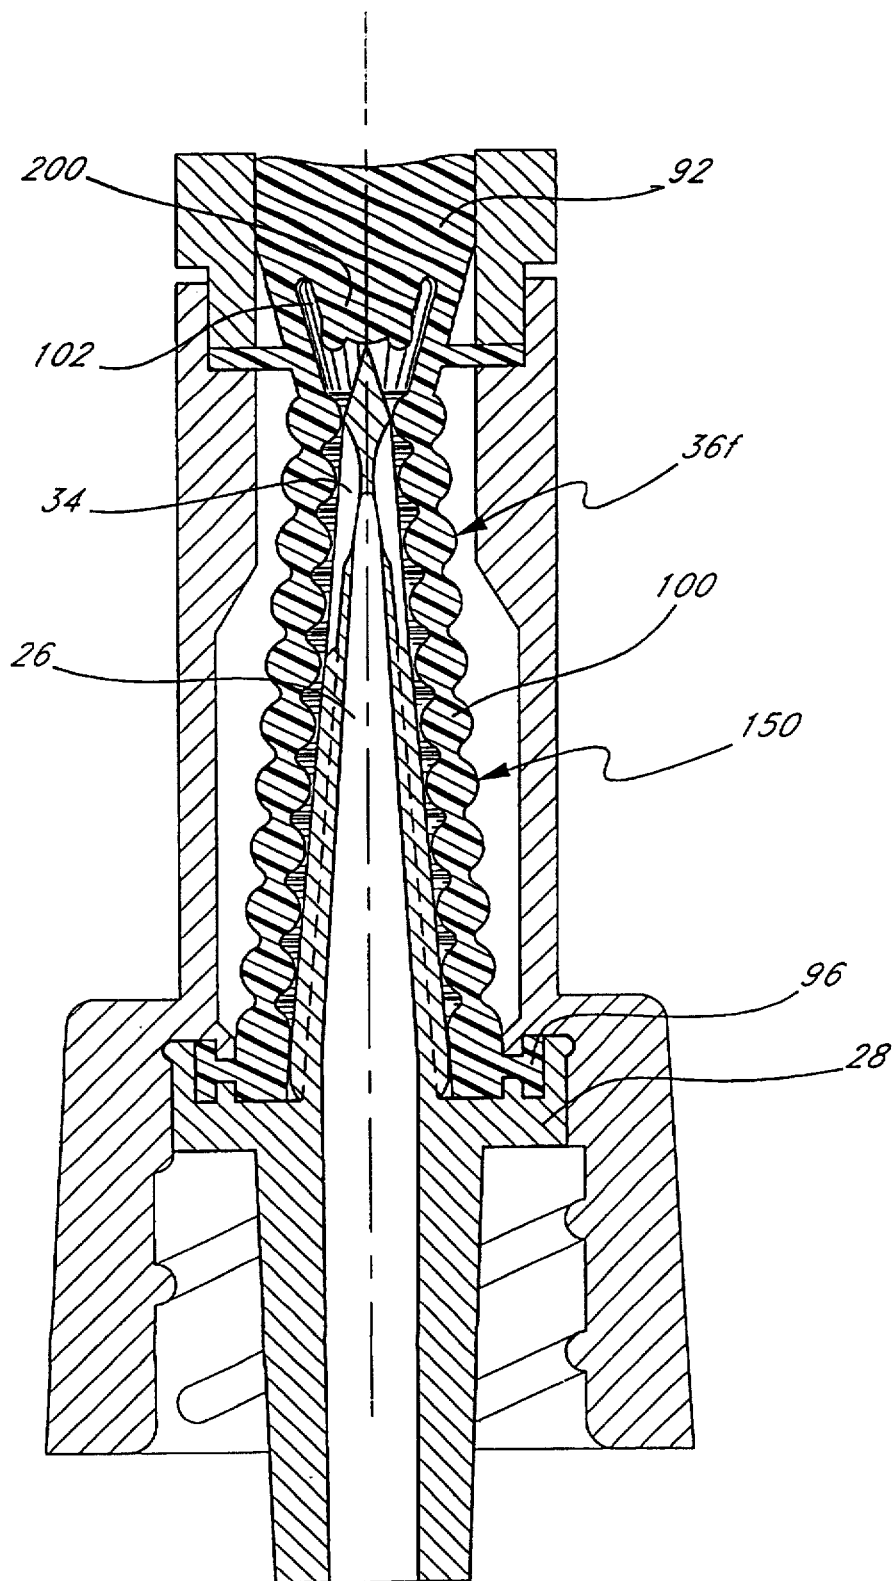


FIG. 17

U.S. Patent

Jun. 3, 2003

Sheet 15 of 19

US 6,572,592 B1

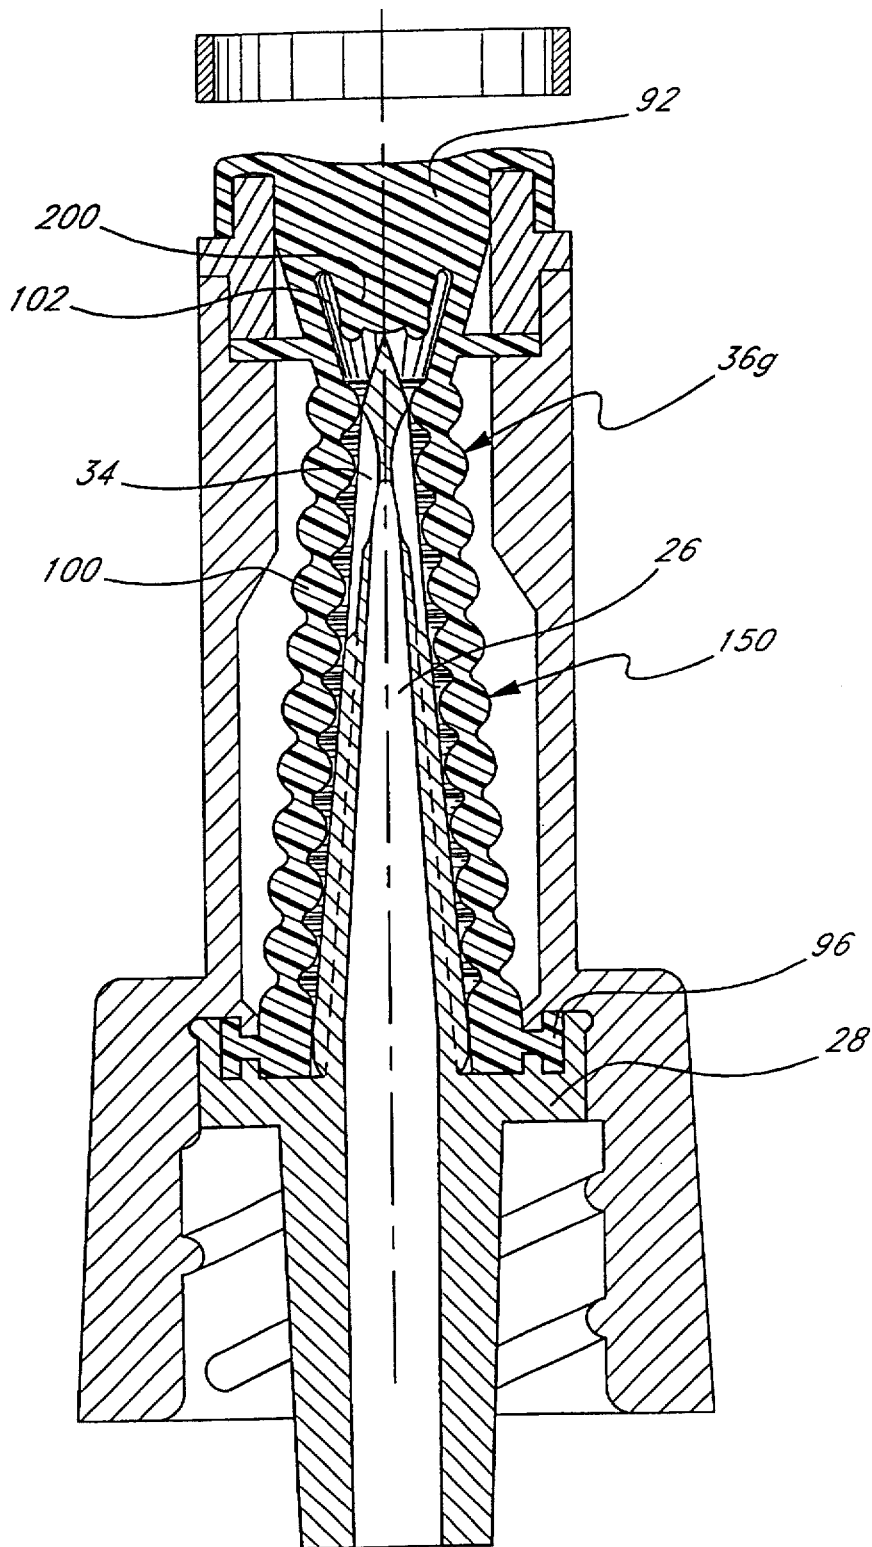


FIG. 18


U.S. Patent

Jun. 3, 2003

Sheet 16 of 19

US 6,572,592 B1

FIG. 19

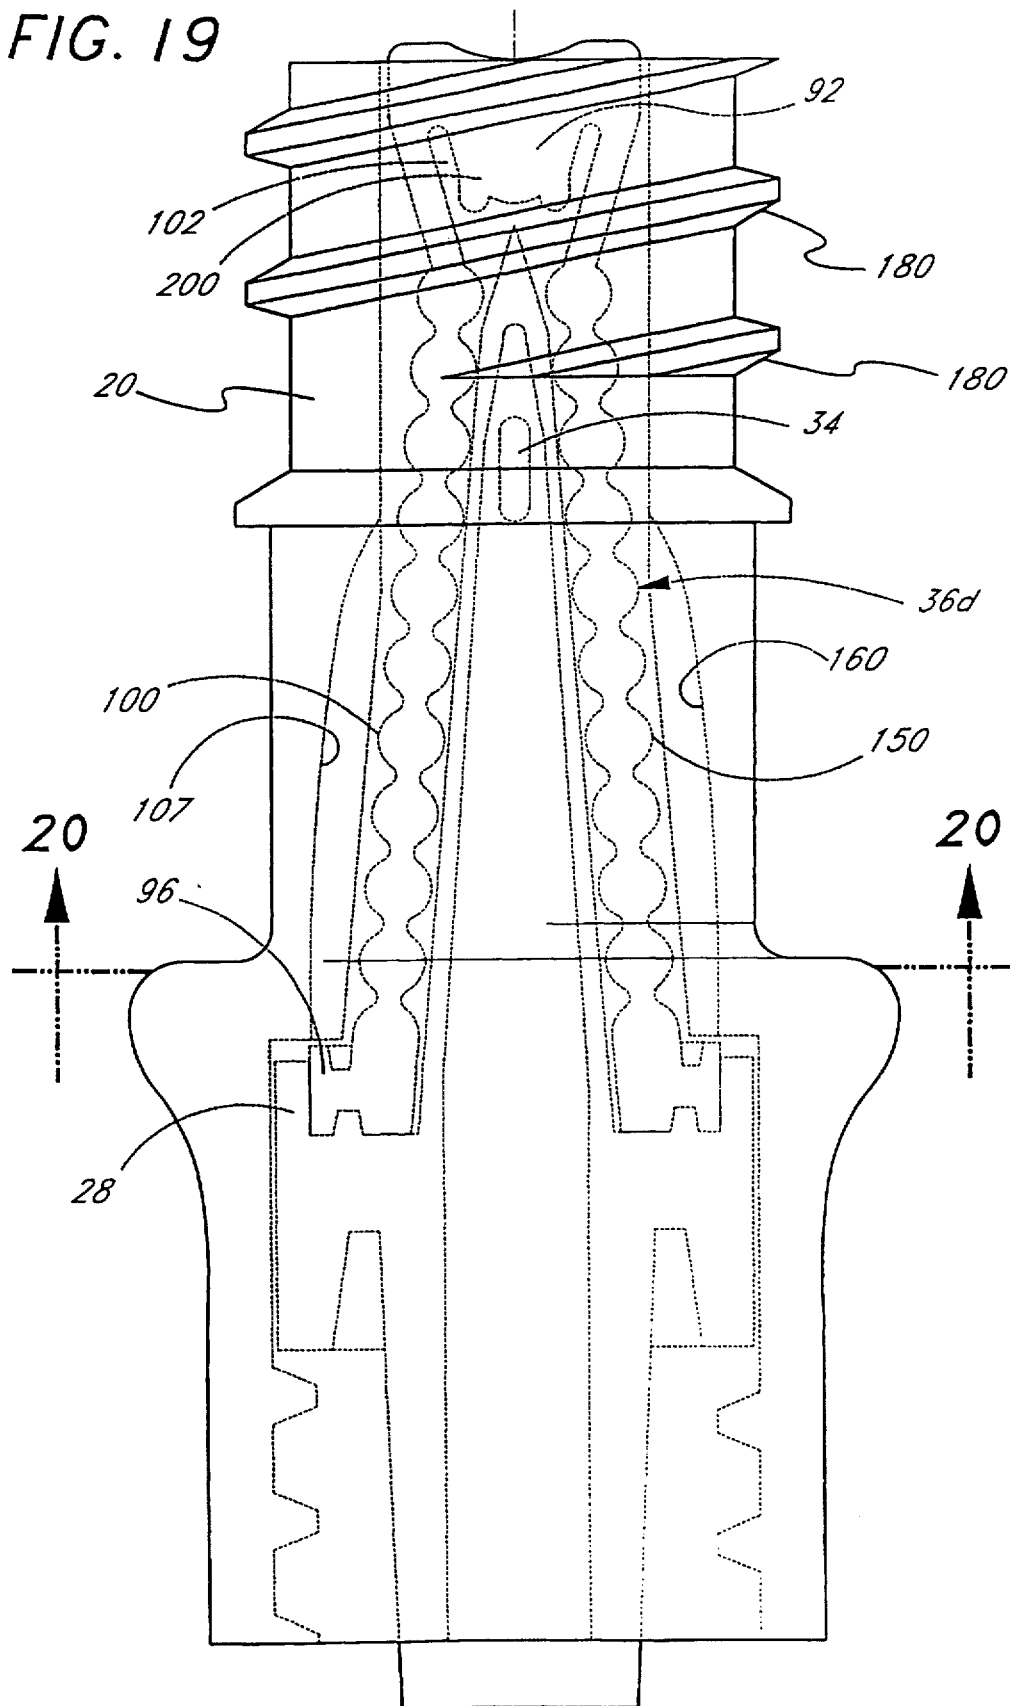

U.S. Patent

Jun. 3, 2003

Sheet 17 of 19

US 6,572,592 B1

FIG. 20


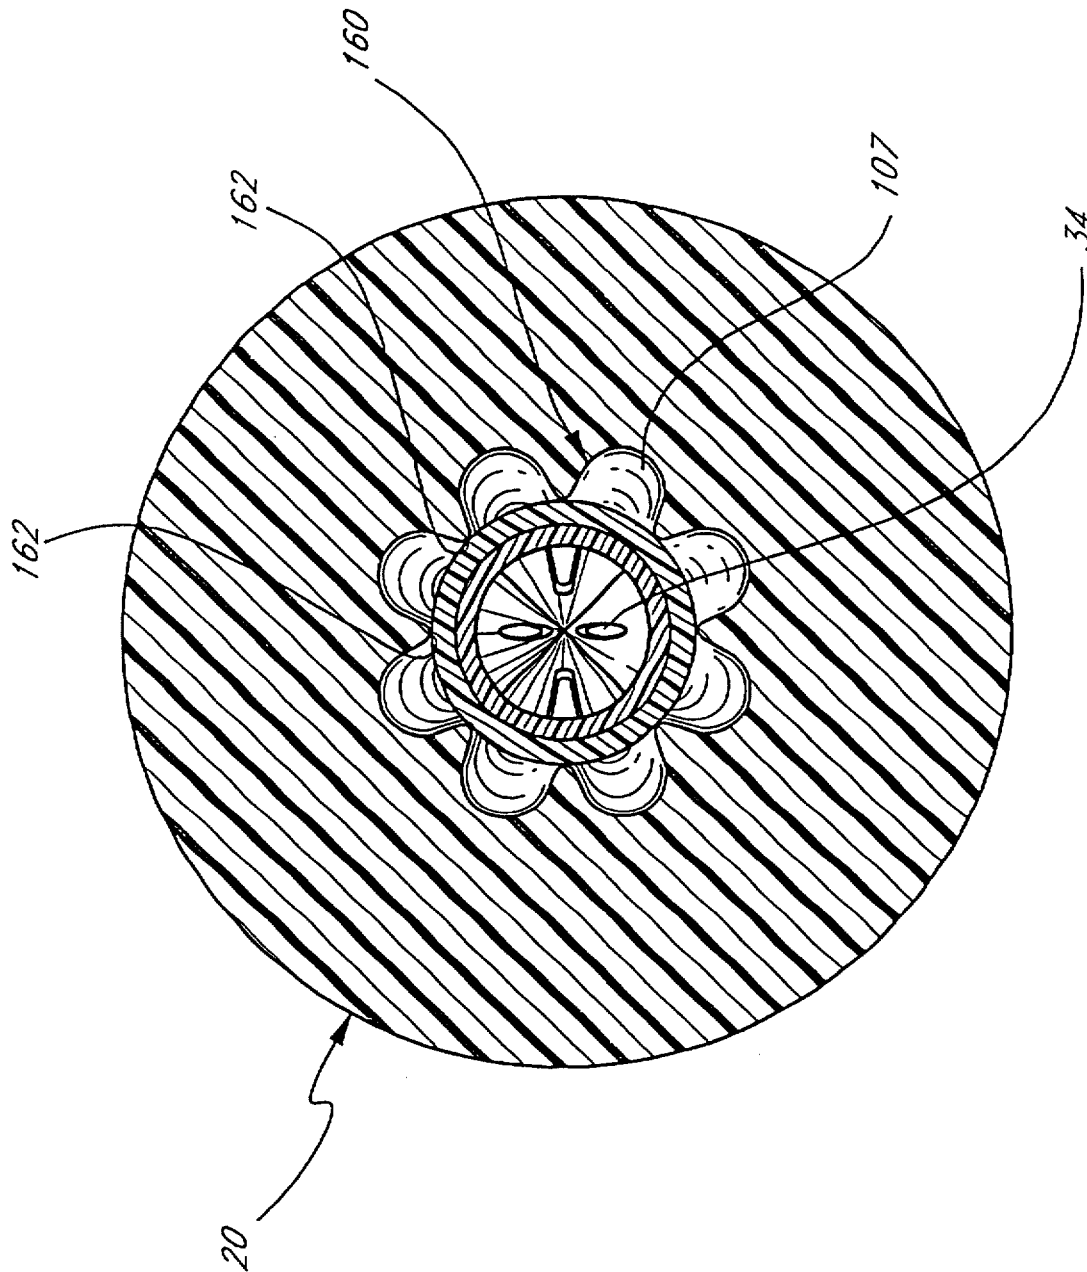


FIG. 21

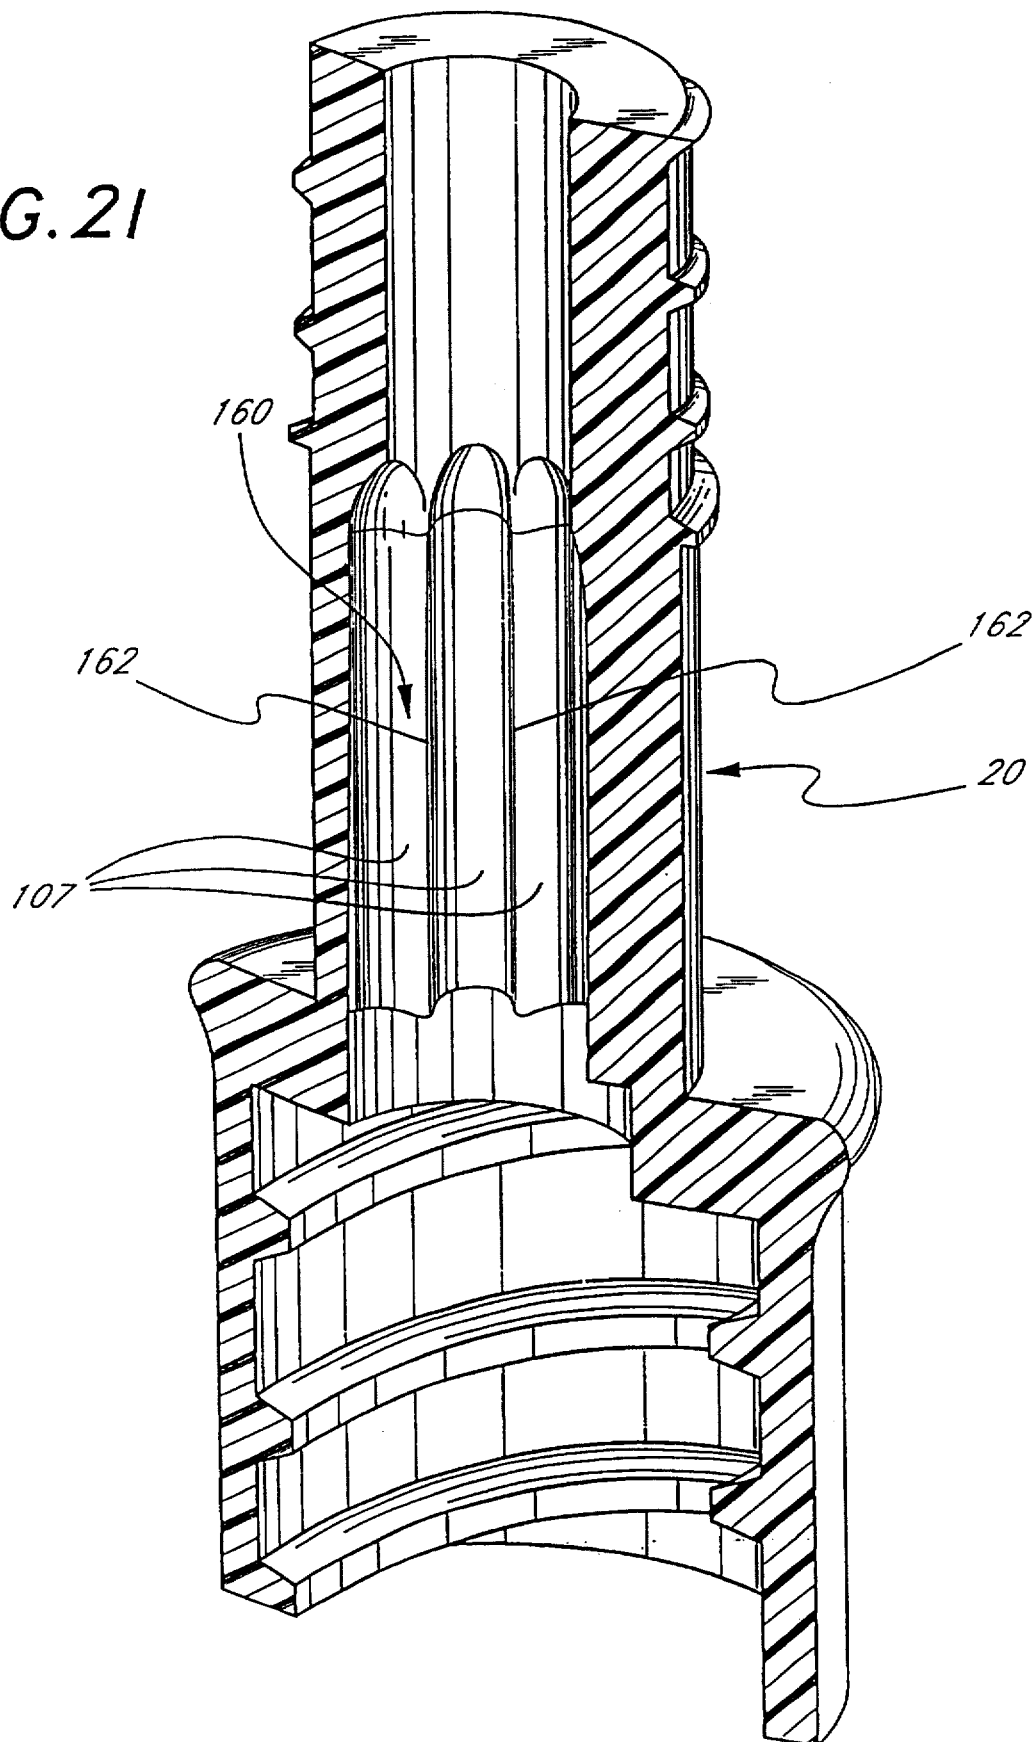


U.S. Patent

Jun. 3, 2003

Sheet 19 of 19

US 6,572,592 B1

FIG. 22

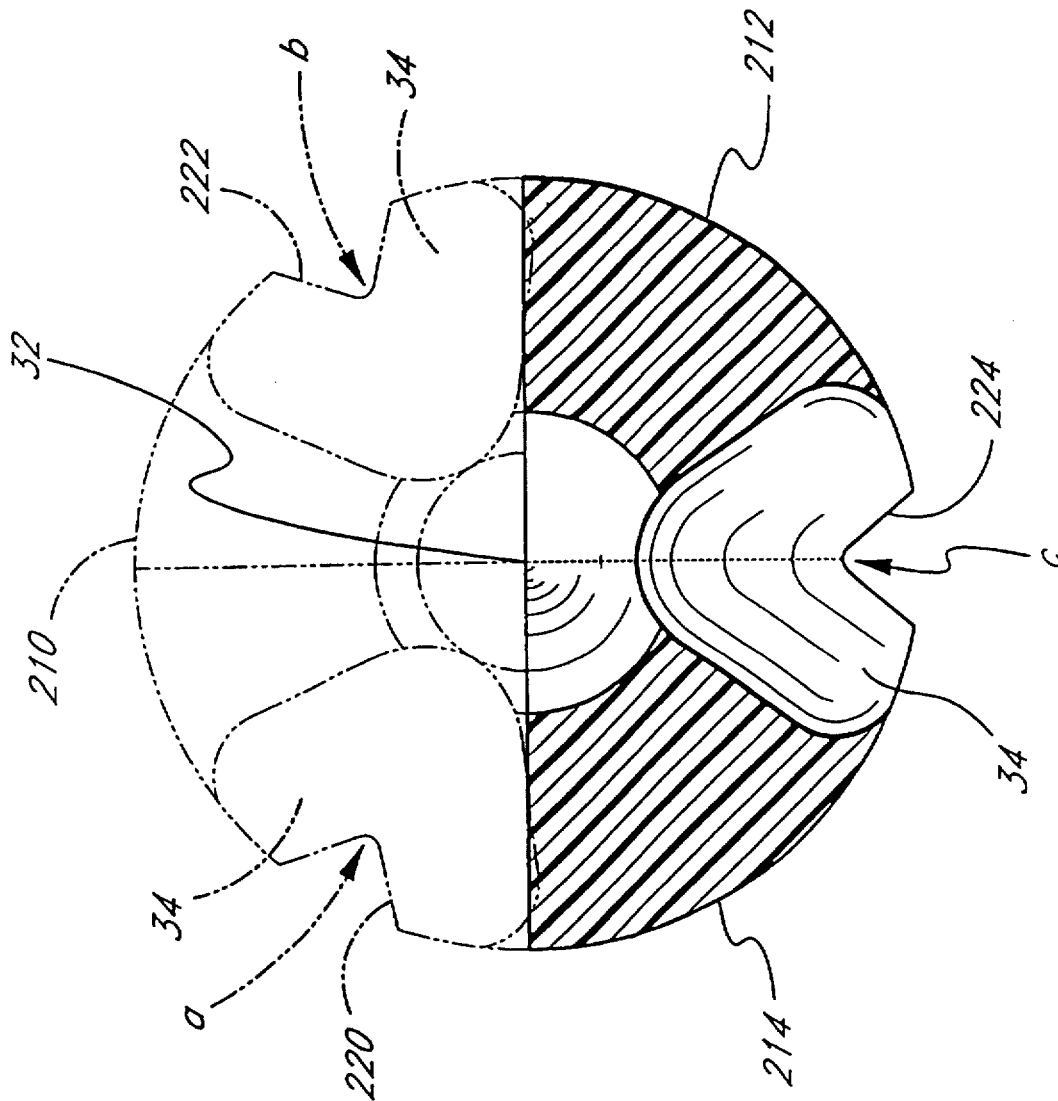

US 6,572,592 B1

1

MEDICAL VALVE AND METHOD OF USE**RELATED APPLICATIONS**

This application is a continuation of prior application Ser. No. 08/905,370, filed on Aug. 4, 1997 now abandoned, which was a continuation of prior application Ser. No. 08/334,846, filed on Nov. 4, 1994 now U.S. Pat. No. 5,685,866, which was a continuation of prior application Ser. No. 08/096,659, filed on Jul. 23, 1993 now U.S. Pat. No. 5,695,466, which was a continuation-in-part of PCT Application No. PCT/US92/10367, filed on Dec. 1, 1992, now abandoned, which was a continuation-in-part of application Ser. No. 07/813,073, filed on Dec. 18, 1991, now abandoned entitled **MEDICAL VALVE AND METHOD OF USE** by inventor George A. Lopez.

BACKGROUND OF THE INVENTION**1. Field of the Invention**

This invention relates to a closed, patient access system which automatically reseals after administering medication using a standard medical implement that directly connects with the system without the need of any intermediary needles, caps or adaptors. A two-way valve eliminating dead space is used which includes a seal which, upon being compressed by the medical implement, is pierced to open the valve and reseals upon being decompressed, maintaining a fluid tight seal even at high pressures and after repeated uses.

2. Background Discussion

The manipulation of fluids for parenteral administration in hospital and medical settings routinely involves the use of connectors and adaptors for facilitating the movement of fluids between two points. Most fluid connectors and adaptors employ needles to pierce a septum covering sterile tubing or to pierce the septum of a medicament container of fluid. Fluid then passes from the container or fluid filled tubing into a syringe or second set of tubing. These connectors and adaptors often have mechanical or moving parts. Since the ready passage of fluids through the connectors and adaptors is often critical to patient survival, it is imperative that the connectors and adaptors function reliably and repeatedly. Adaptors and connectors that malfunction during use may be life-threatening. The more mechanical or moving parts such as springs and diaphragms, the more likely that they will function improperly. Improper functioning can result in the introduction of air embolisms into a patient. Thus, the fewer the mechanical parts, the more these connectors can be relied on and the better they will be accepted by the medical community.

Many connectors or valves, especially those employing several mechanical components, have a relatively high volume of fluid space within them. This "dead space" within the device prevents accurate introduction of precise fluid volumes and provides an opportunity for contamination upon disconnection of the device. Connectors and adaptors often include valves that permit or interrupt the flow of fluid along the course of fluid travel. Several of those commonly in use employ metal needles to puncture sterile seals. Such connectors are generally designed to accommodate fluid flow in one direction. This means that the fluid line must have connectors and tube aligned in complementary directions. These connectors often require further manipulation if, for example, the valve is inadvertently assembled in a direction that will not facilitate fluid flow. These manipulations increase handling, thereby increasing both the risk of contamination and the amount of time required to establish the fluid connection.

2

Metal needles employed as part of connector devices increase the risk of puncture wounds to the user. The needles used in these devices often have through-holes placed at the tip of the needle. Connection of the valve with a flow line involves piercing the needle through a sealed septum. Through-holes placed at the needle tip can core the septum and release free particulates into the flow line. Such an event can prove fatal to a patient. Such through-holes may also become clogged easily with material from the septum.

Reusable connectors and adaptors are preferred for medical applications since components must often be added or removed from a fluid line connected to a patient. Reusable connectors, however, are difficult to keep sterile. Sometimes caps are employed to cover the connector to keep it sterile. Frequently, these caps are lost, or simply not used because they are not readily available when needed.

A closed, patient access system that is easy to use and employs only a valve device in communication with the patient that need not be capped or interconnected with the medical implement through a needle or adaptor, is swappable, is sufficiently durable to maintain its function after several manipulations, and maintains a fluid-tight seal at high pressures, would be of great benefit to the medical community.

SUMMARY OF THE INVENTION

The valve of this invention has several features, no single one of which is solely responsible for its desirable attributes. Without limiting the scope of this invention as expressed by the claims which follow, its more prominent features will now be discussed briefly. After considering this discussion, and particularly after reading the section entitled, "DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS," one will understand how the features of this invention provide its advantages, which include safety, reliable and repeatable performance, elimination of dead space, simplicity of manufacture and use, and employment of a valve that is swappable after use to provide sterility and has a fluid-tight seal at high pressure.

This invention is a closed, patient access system which automatically reseals after administering medication using a medical implement that directly connects with the system without the need of any intermediate needles, caps or adaptors. A two-way valve is employed utilizing a reusable seal that may be repeatedly pierced by an enclosed, protected, non-metallic spike rather than an exposed metal needle. The valve facilitates fluid, particularly liquid, transfer while maintaining sterility. The valve is easy to use and is capable of locking in place. After use, the valve is swabbed in the conventional manner with a suitable substance to maintain sterility. The design of the valve avoids accidental needle sticks. As will be discussed in detail below, the valve is useful as a medical connector or adaptor to enable liquid flow from a sealed container.

The first feature of this invention is that the valve has a body including wall structure defining an internal cavity having a proximal end and a distal end. The cavity has an open space into which the seal is pushed, and preferably has a plurality of radial indentations in the wall structure that are adjacent the seal to accommodate the expansion of the seal upon compression. The proximal end has an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through the delivery end. In most applications, the delivery end of the implement is tapered, and the wall structure, adjacent the opening is tapered inward so that the wall structure and the tapered delivery end

US 6,572,592 B1

3

fit snug against each other upon insertion of the delivery end into the opening. The proximal end of the cavity preferably is adapted to fit snug with an ANSI (American National Standards Institute, Washington, D. C.) standard end of the medical implement. Typically, the implement is a syringe, a connector or inlet/outlet of an IV set, or any one of a wide variety of conduits used in medical applications.

The second feature is that the spike has a tip with at least one hole located at or near the tip, and a passageway in communication with the hole that allows fluid to flow through this hole. The spike is seated inside the cavity such that the tip is inward of the proximal end and is enclosed within the cavity. Preferably, the hole is in a side of the spike adjacent the tip and is elongated, having a size of 18 gauge or greater. The tip may be sharp or slightly rounded. More than one hole is desirable for many applications, and three, symmetrically located holes inward of the proximal end are preferred. The spike may include at least one rib which allows air to enter a space between the seal and the spike, thereby facilitating the sealing of the opening when the implement is removed. The spike may have a substantially conical shape, and the seal has a complementarily, substantially conical shaped cavity within it conforming to the shape of the spike. The spike is disposed within this conical cavity and the seal covers the tip. The tip may be imbedded in the proximal end of the seal or withdrawn into the conical cavity. Preferably, the tip of the spike has a plurality of facets which meet within a recess. The preferred spike should be able to penetrate the seal repeatedly without tearing the seal. Rough edges at the tip may present a tear problem. During injection molding of the preferred plastic spike, facets of the tip will abut along a "parting line," and could form a rough edge which may tear the seal. This problem is avoided where the parting line is buried in a recess. Any rough edge at this parting line is disposed within a recess, so the seal material moves over the recess and does not contact the rough edge.

The third feature is that the resilient seal is adapted to be moved into a compressed state upon insertion of the tip of the medical implement into the opening and returns to a decompressed state upon removal of the tip. The seal in the decompressed state has a section which fills essentially completely a portion of the cavity adjacent the opening. The seal section bears against the wall structure near the opening to seal the opening. In the compressed state, the seal section is pushed by the delivery end of the medical implement away from the opening and into the cavity. A fluid tight seal is maintained between the seal section and the wall structure as the seal is moved into the compressed state. The seal section bears against the wall structure as the seal is moved inward into the cavity by the tip of the medical implement. And most importantly, the delivery end and the seal are adapted to engage so that when the tip of the spike pierces the seal there is essentially no dead space between said delivery end and the seal. Consequently, a predetermined dosage amount of medication is transferred in its entirety to the patient using this invention, with none to the prescribed amount being collected in dead space in the valve. The delivery of an exact amount of medication may be critical in some situations when chemotherapeutic agents are being administered or small children are being treated.

A fluid tight seal is maintained over repeated opening and closing of the valve, and the seal has on its external surface a recess which provides an air pocket to facilitate the movement of the seal. Preferably, the seal presents an essentially flush surface with the proximal end of the cavity. In one embodiment, the proximal end of the seal is substantially flat, the seal is made of a material having a hardness

4

of from 30 to 70 Shore units such as, for example, a silicone polymer. The seal may include a cup-like flange adapted to engage the body near the proximal end of the cavity. A preferred embodiment of the seal comprises a series of O-ring elements stacked together and connected to form a unitary structure. The O-ring elements have increasing diameters, with the smallest diameter element being adjacent the proximal end of the cavity. The proximal end of the seal may be precut to form a tiny orifice therein that allows the tip of the spike to pass therethrough easily upon compression of the seal. Preferably, the proximal end of the seal has a truncated conical shaped segment disposed within the cavity. The seal may also have a centrally located, anti-vacuum, saucer like depression therein, which does not interfere with the ability of the exposed, proximal end of the seal being swabbed when desired.

The fourth feature is that the body and spike are two separate components of the valve that are securely attached to each other by assembly of, and interlocking, of the body and spike. The body has a first locking element near the distal end of the cavity, and the spike has a second locking element adapted to interlock with said first locking element upon assembly. The seal has a lip extending beyond the distal end and positioned between the first and second locking elements so that, upon assembly, the lip is compressed between the locking elements to provide an essentially fluid tight seal upon interlocking.

The fifth feature is that the medical valve includes a support member connected to the spike which seals off the distal end of the cavity. The support member may have a Luer-Lock type connector element that enables the valve to be removably attached to, for example, a fluid line connected to a patient. The support member may also be in the form of an adaptor that enables the valve to be removably attached to a fluid dispenser or container. When used to dispense fluids from a container, the spike has a pair of opposed tips, respectively at the distal and proximal ends of the spike. The tip at the distal end of the spike pierces a cover member which seals the container. A radial slit on the adaptor enables it to deform reversibly sufficiently to fit snugly onto said container.

The sixth feature is that the seal has a proximal end including a pressure responsive element disposed on an inner surface of the seal adjacent the opening. The pressure responsive element in the decompressed state closes any orifice in the seal at the proximal end of the seal to provide an essentially fluid-tight seal while in the decompressed state. The pressure responsive element enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve is connected to a patient's artery. The valve of this invention will remain closed even when the pressure inside the valve is above 6 pounds per square inch (psi), and it can withstand pressures above 30 psi. Typically, the pressure responsive element is a section of the seal having an entryway into a precut orifice. This section has a substantially cylindrical configuration and is surrounded by an annular space which is filled with pressurized fluid. The center of the member and the annular space are coaxial with the entryway to the orifice. The pressurized fluid fills the annular space to apply pressure that compresses the cylindrical section to tightly close the entryway to the orifice. Preferably, the pressure responsive element has an anti-tear element.

In accordance with this invention, a known, prescribed, predetermined amount or dosage of medication may be transferred from the remote source to the patient directly, so

US 6,572,592 B1

5

that essentially none of said predetermined amount is collected in dead space in the valve. In other words essentially all the prescribed dosage is received by the patient and not lost in the valve. Thus, this invention also includes a method of transferring fluid from a remote source to a patient. This invention also includes transfer of fluid from the patient to a remote source. This is possible because the valve of this invention provides two-way communication. The fluid is transferred to the patient by applying pressure the fluid as it passes through the implement so that the pressure applied to the fluid is greater than the pressure of fluid in the patient, enabling transfer from the remote source to the patient. To achieve transfer of fluid from the patient to the remote source, the pressure of fluid in the patient is greater than the pressure at the remote source, causing fluid to flow from the patient to the remote source. This invention also includes a method of transferring fluid in a container having an open mouth covered by a cover member which seals the open mouth. The fluid is caused to flow from the container through the passageway by creating a differential in pressure. Preferably, the valve has an adaptor having a radial slit for allowing the adaptor to deform reversibly sufficiently to fit snugly onto said container.

BRIEF DESCRIPTION OF THE DRAWING

The preferred embodiments of this invention, illustrating all its features, will now be discussed in detail. These embodiments depict the novel and non-obvious method and valve of this invention shown in the accompanying drawing, which is for illustrative purposes only. This drawing includes the following Figures, with like numerals indicating like parts:

FIG. 1 is a perspective view of the first embodiment of the valve of this invention.

FIG. 2 is an exploded perspective view of the valve shown in FIG. 1 illustrating the spike, seal, and the body or housing components of the invention.

FIG. 3 is a longitudinal cross-sectional view of the assembled valve of FIG. 1.

FIG. 4 is a schematic, longitudinal, cross-sectional view of the assembled valve of FIG. 1 before compressing the seal.

FIG. 5 is a schematic, longitudinal, cross-sectional view similar to FIG. 4 showing the valve during compression of the seal.

FIG. 6 is a perspective view of a second embodiment of the invention.

FIG. 7 is a longitudinal cross-sectional view of the valve of FIG. 6.

FIG. 8 is a schematic illustration of an ANSI delivery end of a medical implement compressing the seal of the valve of this invention.

FIG. 9 is a side elevation view, partially in cross-section, of a third embodiment of the seal.

FIG. 10 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using the seal of FIG. 9.

FIG. 11 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fourth embodiment of the seal.

FIG. 12 is a longitudinal cross-sectional view of the assembled valve of FIG. 1 using a fifth embodiment of the seal.

FIG. 13 is a longitudinal cross-sectional view of a sixth embodiment of the seal.

6

FIG. 14 is a longitudinal section of the seal shown in FIG. 13 used in connection with the spike device shown in FIG. 2.

FIG. 15 is a longitudinal partial cross-sectional view of a seventh embodiment of the seal of this invention,

FIG. 16 is a longitudinal cross-sectional view, after assembly, of the embodiment of the valve shown utilizing the seal of FIG. 15.

FIG. 17 is a longitudinal cross-sectional view, after assembly, of the eighth embodiment of the valve of this invention.

FIG. 18 is a longitudinal cross-sectional view, after assembly, of the ninth embodiment of the valve of this invention.

FIG. 19 is a side elevation view, after assembly, of the seal and spike shown in FIG. 14 connected to the body or housing shown in FIGS. 20 and 21.

FIG. 20 is a cross-sectional view taken along line 20—20 of FIG. 19.

FIG. 21 is a perspective view, with sections broken away to show the wall structure of the cavity containing the seal shown in FIGS. 13 and 14.

FIG. 22 is a greatly enlarged, cross-sectional view taken along line 22—22 of FIG. 14.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

The term “proximal” is used to denote the end of the valve and other components at or near the spike tip 32 in FIGS. 2 through 5, 10 through 12, 14, and 16, and at or near the spike tip 60 in FIG. 6, and at or near the seal cap 92 in FIGS. 8, 9, 13 through 19. The term “distal” is used to denote the opposite end of the valve, or spike tip, or seal. The term “medical implement” is used to denote any medical tool known to those of skill in the art that can connect to the present invention and facilitate the passage of fluids, particularly liquids, through the instant invention. Examples of medical implements that are contemplated include, but are not limited to, tubing, conduit, syringes, IV sets (both peripheral and central lines), piggyback lines, and other components which can be used in connection with a medical valve. Medical implements are commercially available in standard sizes. Thus, either or both ends of the valve of this invention can be provided with fittings to accommodate such standard size medical implements.

As best shown in FIGS. 1 and 2, the first embodiment of the invention, valve 10, includes a valve body or housing 12, a spike element 24, and a seal 36. The seal 36 is prepared from a resilient material that is flexible, inert, impermeable to fluid, and readily pierceable by the spike 26. In the embodiment shown in FIG. 13 depicting an alternate shaped seal 36d, this seal 36d has a precut slit 11 in its proximal end. This provides a tiny orifice through which the tip 32 of the spike element 24 may easily pass, yet still provides a fluid tight seal upon withdrawal of the spike element. These three components are assembled, as depicted in FIG. 3, with the spike element 24 enclosed to prevent accidental sticks. FIG. 2 illustrates how the housing 12, seal 36, and spike element 24 are attached without the need to use any adhesive or other bonding agent or process. Mechanical connection which provides a fluid tight closure is attained as is discussed subsequently. As shown in FIGS. 4 and 5, the seal 36 moves within the housing 12, being pierced by the spike element 24 to expose the tip 32 of the spike element 24 to allow fluid to flow through the valve 10.

US 6,572,592 B1

7

Referring to FIG. 1, one preferred embodiment of housing 12 has a bell-shaped skirt 16 and an upper, preferably cylindrical, conduit 20. The skirt 16 is integral with, and connected by an annular ring 14, to the upper conduit 20. The skirt 16 creates a shield for an inner conduit 18 of the spike element 24. This inner conduit 18 is preferably cylindrical in shape, and slightly tapered. Inner conduit 18 and upper conduit 20 comprise aligned hollow tubes so that inner conduit 18 and upper conduit 20 are in fluid communication with one another when the spike element 24 pierces the seal 36. There is an annular lip 25 surrounding a circular opening 25a in the top of the conduit 20 (see FIG. 2).

In the first embodiment, the upper conduit 20 is adapted to receive the tip or nose 48 of an ANSI standard syringe 46 (see FIGS. 4 and 5). It is, however, contemplated that the outer diameter of the upper conduit 20 can be of any size to accommodate the attachment of other connector devices thereto. Advantageously, the proximal end of the upper conduit 20 can be equipped with a locking mechanism to facilitate locking of the valve 10 to a variety of connector devices. For example, referring to FIG. 1, locking ears 22 near the proximal lip 25 of housing 12 are preferably provided such that the housing 12 can be locked into any compatible Luer-Lock device known to those with skill in the art. For example, referring to FIG. 19, conventional Luer-Lock threads 180 can be provided on the outer diameter of upper conduit 20.

Referring to FIG. 2, the spike element 24 has at its distal end the inner conduit 18 and at its proximal end a hollow spike 26 which is integral with the inner conduit. The inner conduit 18 and spike 26 present a continuous passageway for fluid during use. An annular cuff 28 on an intermediate portion of the spike element 24 is integral with, and interconnects, the inner conduit 18 and the spike 26. As illustrated in FIG. 3, the rim 28a of the cuff 28 abuts the underside of the inner ring 14, and has an annular detent 28b that snaps into an annular groove 14b in the underside of the ring. The cuff 28 serves two functions. First, it serves as an attachment device to the underside of the annular ring 14. Second, it serves as a support and attachment device for the seal 36.

The hollow spike 26 has a tapered conical shape, ending in a sharp, pointed tip 32. Preferably, along the length of the spike are raised, protruding ridges 30. These raised ridges 30 extend from the surface of the spike preferably between 0.2–2.0 mm. The ridges 30 are preferably aligned along the length of the spike as illustrated in FIG. 2. These ridges 30 serve to break any vacuum created when the spike 26 is sealed as described hereinbelow. Modifications to the alignment and orientation of the ridges are discussed hereinbelow in association with their function. Just distal the spike tip 32, there is situated at least one longitudinal through-hole 34 to permit fluid communication between the inner conduit 18 and the upper conduit 20. Preferably, there are three through-holes 34 within about 0.200 inch from the spike tip 32. These through-holes 34 may be of any size, however, the larger the size of the through-holes the greater the fluid flow rate through the valve 10. In a preferred embodiment, the size of the through-holes 34 are 18-gauge to provide a flow rate three times that of a standard 18 gauge needle.

The seal 36 has a seal cap 40 with a generally flat top surface 40b, an outwardly tapered sidewall 38, and a lower lip 42. Its interior is hollow to provide the conically shaped cavity 37 (FIG. 3). Thus, the seal 36 slips easily over the spike element 24 to fit snugly within the cavity 37. The seal lip 42 is seated within the annular cuff 28 and wedged between the cuff and the underside of the ring 14. There are

8

longitudinal grooves 43 (FIG. 2) along the length of the seal 36 which provide air pockets that facilitate compression of the seal 36 during use. The grooves 43 may be of variable shape or size to facilitate seal compression. In the first embodiment, there is a single groove 43 which completely surrounds the seal 36 between the seal cap 40 and the lip 42.

The base of the seal 36 has a width such that the seal lip 42 fits snugly into the annular cuff 28. The hollow interior or cavity 37 (FIG. 3) of the seal 36 is preferably tapered to conform internally to the shape of the spike 24, having a wall portion 44 which contacts the spike 24 distal seal cap 40. The exterior of the seal 36 is sized and shaped to fit inside the upper conduit 20 of the housing 12. The cap 40 reseals the valve 10 when the top surface 40b is above the through-holes 34. Preferably, the cap 40 substantially fills the opening 25a in the top of the conduit 20. Thus, after assembly, the top surface 40b of the seal cap 40 is essentially flush with the lip 25, so that the lip 25 and seal cap 40 can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve 10. It is important that the surface 40b be exposed so that it may be swabbed with a disinfectant.

As best shown in FIG. 3, the spike 24, with contiguous inner conduit 18, is affixed to the housing 12 through the association of the external portion of annular cuff 28 and the internal portion of annular ring 14. Although not necessarily required, these two pieces may be affixed by any one of a variety of methods known to those of skill in the art including, but not limited to, heat sealing, glue, pressure lock, bonding or the like. The seal 36 fits into the annular cuff 28 and is held in place by an internal lip 27 along the internal portion of the annular ring 14 of the housing 12. The length of the spike 24 is such that, after assembly, the tip of the spike rests below the plane defined by the lip 25 of the housing 12. Preferably, the spike tip 32 is approximately from 0.525" to 0.1" below the lip 25 of the housing 12. The seal 36 fits snugly against the spike 24 and is essentially flush with the lip 25 of the housing 12. The spike tip 32 is thus embedded within the seal cap 40 prior to use or may be approximately 0.025" distal the seal cap 40 when the valve 10 is in the closed position. The inner conduit 18 is partially shielded by the bell shaped skirt 16 of the housing 12 (see FIGS. 1–3). The inner surface of the bell shaped skirt 16 preferably has protruding threads 44 as an optional locking mechanism for attaching a medical implement thereto. Further, other medical devices can be pressure fit over the outer portion of inner conduit 18 without direct association with the protruding threads 44.

During use, the invention is designed to be adapted as a two-way valve. The orientation of the valve is independent to fluid flow and dependent on the preferred orientation of the preexisting connections. Thus, the invention can be used as a valve connector for an intravenous central or peripheral piggyback connector in either orientation. Parenteral fluid is delivered to patients through tubing such that the liquid flows from a container through a needle into the patient. The containers are frequently changed or additional fluid bottles are added. The invention disclosed herein is designed to interconnect medical implements along the route of fluid delivery to the patient. However, the invention is also useful in any environment in which a resealable fluid valve is desired. During use, a connector of the appropriate size is fitted over the inner conduit 18. Locking can be achieved by a Luer-Lock mechanism, a pressure fit or any other locking mechanisms known to those with skill in the art, as described above. Thus, in one example, fluid passes from the inner conduit 18 into the spike 26. However, fluid flow is locked in place by the seal 36.

US 6,572,592 B1

9

FIGS. 4 and 5 illustrate valve activation. In FIG. 4, the medical implement connecting to the proximal end of the valve 10 is a syringe 46. However, this connecting implement could be any number of medical implements known to those of skill in the art. The nose 48 of the syringe 46 is placed on the seal cap 40 inside the lip 25 of the housing 12. The application of pressure on the syringe 46 in the direction of the arrows, as illustrated in FIG. 4 creates pressure on seal cap 40. The resulting downward pressure compresses the seal 36. This pushes the tip 32 of the spike 26 through the seal cap 40 to expose the through-holes 34. Compression is facilitated by the grooves 38. Fluid is now able to flow into the syringe 46, or vice versa, depending on whether fluid is to be withdrawn from the patient or medication injected into the patient. FIG. 5 shows valve 10 opened by insertion of the nose 48 of the syringe 46 into the opening 25a. A syringe plunger 49 in the syringe 46 is retracted thereby creating a vacuum to draw fluid through the valve 10 into the syringe. For intravenous applications, the valve 10 can be orientated in the position diagramed in FIGS. 4 and 5, or it can be rotated 180° such that fluid flows in the opposite direction.

Upon removal of the syringe from spike 26, as shown in FIG. 4, the seal 36 is free to return to its original shape and cover through-holes 34. The ability of the seal 36 to return to its original shape is determined by the resiliency of the material used to prepare the seal 36. In addition, the ability of the seal 36 to return to its original shape is facilitated by the protruding ridges 30 formed on the external surface of the spike. During compression, a vacuum may form in the area between the spike 26 and the seal 36, thereby preventing the seal 36 from returning to its original position. The protruding ridges permit air to pass along the spike/seal interface to prevent vacuum formation and allow free return of the seal. The ability of the seal 36 to deform reversibly and return to its original position is particularly useful because (1) it immediately stops fluid flow through the valve 10, (2) it covers the recessed spike 26 to maintain its sterility, and (3) it reduces the risk that the spike could inadvertently pierce another object or person. In addition, since the valve 10 lacks movable parts, except for the seal, it is unlikely that when the seal 36 is pushed down, the valve 10 would fail to function.

Advantageously, the through-holes 34 are located relatively low on the spike 26. Thus, the through-holes 34 are sealed relatively early in the process as the seal 36 returns to its original configuration with the valve 10 is closed. In one preferred embodiment the through-holes 34 are located 0.075" below the spike tip 32 (see FIG. 2). Additionally, the through-holes 34 are sealed even if the seal 36 does not fully return to its original configuration depicted in FIG. 4. Further, the ability of the seal 36 to return reversibly to its original position permits the reuse of the connector valve 10. Following disconnection, and before reuse, the surface of pierced seal cap 40 is essentially flush with the housing 12. Thus, this flush surface can, advantageously be sterilized with alcohol or other surface decontaminating substances. The skirt 16 and upper conduit 20 advantageously shield both connections from the surrounding environment to protect the sterility of the connection. Further, both the skirt 16 and upper conduit 20 function as collection reservoirs to prevent fluid from dripping from the valve 10 during manipulation.

A cover cap (not shown) can be supplied to fit over the upper conduit 20 as further protection for the seal surface between use. Such a cover cap, however, is not needed to maintain sterility since the seal 36 may be swabbed with a disinfectant after each use. The reversibility of the seal 36

10

makes the valve 10 particularly attractive as a connector valve to provide fluid communication between two fluid lines. Therefore, the present invention provides for placing a first fluid line in communication with a second fluid line using the valve disclosed herein. The reversibility of the valve 10 permits multiple fluid lines to be successively added, for example, to a fluid line in direct communication with a patient's vein. Since the valve is easily sterilizable and sealable, fluid lines can be added and removed without disconnecting venous contact.

The valve 10 is preferably prepared from a hard plastic, but it is additionally contemplated that the valve could be prepared from other medically inert materials known to those in the art. The spike element 24 is preferably prepared from the same material as the housing 12. One particular advantage of this invention is that it does not rely on the use of metal needles. This dramatically reduces the risk of skin puncture during use and manufacture. Further, the upper conduit 20 serves as a shield to the spike 26 such that skin puncture is further reduced. The spike 26 need only be strong enough to penetrate the seal cap 40, or if necessary, to pierce a connecting septum.

In the embodiment of the invention illustrated in FIGS. 2-4, the through-holes 34 are placed distal spike tip 32. This placement provides two important advantages. First, the placement of the through-holes 34 facilitates resealing of the valve 10 after use. Second, if the through-holes were placed at the spike tip 32, the holes 34 may core the seal cap 40 thereby introducing seal particulate into the fluid flow and possibly plugging the holes 34. Thus, the longitudinal placement of the through-holes distal spike tip 32 prevents the introduction of particulates into the fluid path and/or plugging of the through-holes 34. It is additionally contemplated that the number and diameter of the through-holes 34 can be adjusted to accommodate different fluid velocities. In a preferred embodiment, the preferred velocity of fluid passing through the through-holes 34 is equal to or greater than the flow rate through an 18 gauge needle. Through-holes larger than 18 gauge will, of course, facilitate greater fluid velocities.

An important advantage of the invention is that the valve 10 has very little dead space, thus the volume of liquid entering into the valve is substantially equivalent to the volume of fluid leaving the valve. Further, the total equivalent fluid volume of the valve is very small such that the volume of fluid flowing through the system in order to place the valve in fluid communication with a medical implement such as a syringe 46 is substantially zero.

Alternate Embodiments

In another preferred embodiment of the invention, illustrated by FIGS. 6 and 7, a disposable sterile adaptor valve 50 is provided to function as a resealable lid for a container (not shown) of fluid. The fluid can thus be removed from the fluid container or permitted to flow from the container into a medical implement adapted to house fluid in a sterile manner. As is the conventional practice, an open mouth of the container will ordinarily be sealed with a cover member (not shown).

FIG. 6 shows an adaptor valve 50 having a body including an adaptor skirt 52. The adaptor skirt 52 will preferably fit snugly over the open mouth of the container. The skirt 52 may be of any size to accommodate a range of container sizes. A lengthwise slit 54 is preferably provided in at least one location along the length of the skirt to ensure a snug fit between the skirt 52 and the container. A chamber 56,

US 6,572,592 B1

11

preferably tubular in configuration, extends upward from the skirt 52 and is similar in construction and design to the upper chamber 20 of the first preferred embodiment. Similar to the first embodiment, the proximal portion of the valve contains a locking mechanism 59 that preferably comprises a Luer-Lock device or other locking device known to those of skill in the art.

As depicted in FIG. 7 a spike 58 extends upward through a tubular chamber 56. A spike tip 60 is preferably recessed from a proximal lip 62 of the tubular chamber 56. In a closed position, this tip 60 is covered by a seal 64, which is essentially the same as seal 36. Protruding ridges 66 and seal grooves 68 facilitate seal compression in the open position and promote closure following use. Thus, in the closed position as illustrated in FIG. 7, the seal 64 covers the through-holes 70 to prevent fluid out-flow from the container. The adaptor valve 50 contains a second spike 72 which points in the opposite direction as spike 58. These spikes 52 and 72 are in fluid communication with each other. The spike 72 extends downward inside the adapter skirt 52. The two spikes preferably form one component of the valve 50 while the skirt 52 and upper chamber form a second component. These two components can be assembled in a manner like that of the valve 10. The spike 72, like the spike 58, has longitudinal through-holes 74 and a tip 76. The through-holes 74 are located inward of the tip 76. The adaptor valve 50 is thus useable with containers holding sterile medicament having a cover or septum seal at the open mouth of the container. Examples of containers with such seals contemplated for use with this invention include dosage bottles for intramuscular injector antibiotic containers or the like. However, it is also contemplated that the valve 50 can be adapted with its own seal and locking mechanism to permit the valve to be employed on a variety of containers for medicaments or other fluids. Medicaments in these types of containers are preferably maintained under sterile conditions and the volume and nature of the medicament is such that multiple aliquots are intermittently removed over time. If the medicament is reconstituted, then, during use, any covering over the opening on the container is removed to reveal the rubber septum. The adaptor valve 50 is placed over the septum and direct pressure is applied to pierce distal spike 72 through the septum and into the container. A syringe or the like can then be applied, as depicted in FIG. 4, in association with the first preferred embodiment, to withdraw fluid from the container. The pressure of the nose 48 over the spike 58 pushes spike tip 60 through seal 64. At the same time, seal 64 is pushed back and compresses. Compression is accommodated by seal grooves 68. Fluid is withdrawn from the container and the syringe is removed from the spike 58. Release of the pressure applied to seal 64 permits the seal to return to its original configuration. The spike ridges 66 facilitate seal reversibility.

Often the ingredients housed in containers are those that can be lyophilized at purchase. Lyophilized ingredients require reconstitution before use. If the medicament requires reconstitution before use, then sterile water, saline, or other fluid can be introduced into the container before fluid is extracted. The two-way nature of the valve permits this without any special adaptation. After the syringe is removed, the adaptor valve 50 automatically seals. Subsequently, aliquots can be removed from the container by syringe or the like. Alcohol or other compatible surface sterilizing agent can be used to wipe the lip 62 and seal 64 before each use. Similar to the first embodiment, it is additionally contemplated that a cap can be provided to fit over upper chamber lip 62 between use.

12

The adaptor valve 50 can be adapted to function as a medicament adaptor for an intravenous container. In this case, the adaptor valve 50 is placed on a medicament container for intravenous delivery and attached via tubing to an intravenous feed. Thus, the adaptor valve 50 can be placed in fluid communication with a connector valve of FIG. 1 to facilitate the flow of medicament from intravenous drip bottles.

An alternative embodiment of the seal, a seal 36a, is shown in FIG. 9. Seal 36a comprises a seal cap 92 at the proximal end thereof and a seal lip 96 at the distal end thereof. A cup-like annular flange 95 is provided proximal seal cap 92. The seal cap 92 and seal lip 96 are connected by a seal wall consisting of a plurality of ringed wall portions 94 that expand and collapse in an accordion like fashion. During compression of the seal 36a, the diameter of the ringed wall portions 94 expand outward in the radial direction. There are air pockets 13a (FIG. 10) between ring portions 94 and the housing and air pockets 13b between spike 24 and seal 36a. The seal 36a contains a cavity 98 distal seal cap 92 and adjacent the ringed wall portions 94. The seal 36a interacts with spike 26 (FIG. 2) and other components of the present invention in a similar fashion to seal 36 of FIG. 2.

Referring to FIG. 10, the cup-like annular flange 95 may be stretched around the upper conduit 20 and held in place by an annular ring 97. This creates a trampoline like effect that assists returning the seal 36a to a decompressed state after withdrawal of a syringe (not shown). This embodiment has two advantages. First, the proximal end of the valve 10 can be swabbed with alcohol or other disinfectant without leakage of disinfectant into the valve 10. Second, by affixing cup-like annular flange 95 to upper conduit 20 at the proximal end thereof with annular ring 97, the repeated deformation and reformation of the seal 36a is assisted.

An alternative embodiment of the seal, a seal 36b is shown in connection with the valve 10 in FIG. 11. The seal 36b is similar to the seal 36a and is comprised of seal cap 92, a side wall consisting of ringed wall portions 94 and a seal lip 96. It also has an outwardly extending ring 99 which is at a right angle with respect to the longitudinal axis of the valve 10. This ring 99 is used to attach the seal 36b to upper conduit 20. Preferably, an upper conduit annular plug 20' is inserted within upper conduit 20 to create a tight fit between perpendicular ring 99, a ledge 101 in the upper conduit 20, and the plug 20'. The ring 99 assists in the reformation of seal 36b to enclose spike 26 upon withdrawal of a syringe (not shown).

As shown in FIG. 12, the cup-like annular flange 95 and ring 99 may both be used in connection with the valve 10, to provide the seal 36c. This seal 36c, provides rapid reformation upon withdrawal of a syringe (not shown) and realizes the advantages of both the seals 36a and 36b.

Another alternative embodiment of the seal, a seal 36d, is shown in FIG. 13. In this embodiment, the seal 36d is comprised of seal cap 92, seal lip 96, and a side wall 150 comprised of circular tires 100 stacked in series one on top of an adjacent larger diameter lower tire. The circular tires 100 are preferably solid throughout the diameter of the cross-section thereof. These circular tires 100 will deform and reform upon, respectively, compression and decompression of the seal 36d, thereby exposing or covering a spike (not shown) as the case may be.

As mentioned above, preferably seal 36d has a precut slit 11 in the cap 92 lying along the longitudinal axis of the valve 10. The seal cap 92 has a unique configuration that insures

US 6,572,592 B1

13

that the slit 11 closes and is sealed upon withdrawal of a syringe (not shown) and reformation of the seal 36d. It includes an enlarged, internal, pressure responsive member 200 which is integral with the cap 92. Between the proximal end of the side wall 150 and the member 200 is an annular space 102 which is filled with the fluid in the cavity 98. This fluid is under pressure, for example at the blood pressure of the patient to which the valve 10 is attached. Referring to FIG. 14, fluid, for example the patient's blood, flows through the holes 34 in the spike 26, filling the cavity 102. This fluid presses against the exterior of the member 200, closing the slit 11 when the seal is decompressed as shown in FIGS. 14 and 19. The pressure from this fluid creates a high pressure seal which prevents fluid from escaping valve 10 through the slit 11. There is a semi-cylindrical annular flange tear ring 104 on the end of the member 200 which advantageously extends the useful life of seal 36d.

Preferably, there is a tear ring 104 integral with the member 200 along the perimeter of the internal surface the member 200, and a slight saucer-like depression 204 in the external surface of the seal. The pressure responsive element in the decompressed state closes any orifice in the seal 36d to provide an essentially fluid-tight seal while in the decompressed state. The pressure responsive member 200 enables the valve to maintain a fluid-tight seal even at very high pressures sometimes experienced in medical applications, particularly when the valve 10 is connected to a patient's artery. The center of the member 200 and the annular space 102 are coaxial with the entryway 11a to the orifice 11. The pressurized fluid fills the annular space 102 to apply pressure that compresses the member 200 to tightly close the entryway to the orifice. In a preferred embodiment the distance from the entryway 11a to the proximal end of seal cap 92 is from 0.500 to 0.075 inches and more preferably approximately 0.100 inch.

As best illustrated in FIG. 22, the tip 32 is designed to avoid tearing the seal. Tip 32 has three facets 210, 212, and 214 which are joined with each other along parting lines a, b, and c. This junction of the facets 210, 212, and 214 frequently is ragged and will tear the seal 36d. This is prevented by the parting lines a, b, and c, or junctions, being disposed within recesses 220, 222, and 224, respectively, to provide "buried parting lines."

Another alternative embodiment of the present invention using the seal 36d is shown in FIG. 8 and FIGS. 19 through 21. In this embodiment, the inner wall 160 of the upper end of the conduit 20 is provided with at least one, and preferably, a plurality of radial indentations 107. The indentations 107 are elongated disposed generally parallel to the longitudinal axis of the valve 10 in a symmetrical, star-like configuration. Each indentation has opposed lateral edges 162 which engage the seal 36d upon compression of the seal 36d. The indentations provide space into which the seal 36d expands upon compression.

As best shown in FIG. 8, the wall 181 of the proximal end of the conduit 20 is tapered inward at the same angle as the nose 48 of the syringe 46. In accordance with ANSI standards, the taper is 0.006 inch per linear inch. The wall 182 of the syringe nose 48 bears against the wall 181 as the nose slides into the opening 25a to push the seal 36d inward compressing it and forcing the tip 32 of the spike 36 to enter the slit 11. The seal 36d expands upon compression to fill essentially completely the upper portions of the indentations 107. Some sections of the seal 36d are wedged between the edges 162 and other sections fill the indentations 107. As the liquid flows through the nose 48 through holes 34, air in the nose 48 is forced out of the nose 48 and expelled from valve

14

10 between walls 181 and 182. Thus, essentially the entire prescribed dosage is delivered through valve 10 to the patient. Fluid flows through the through-holes 34, but does not leak between either the seal 36d and the wall 181 or between the abutting walls 181 and 182.

FIGS. 15, 16, 17, and 18 depict embodiments of seals, namely, seal 36e, seal 36f, and seal 36g, which are substantially the same as the seals 36a (FIG. 10), seal 36b (FIG. 11), and seal 36c (FIG. 12), except the side wall 150 employing the circular tires 100 is used in place of the accordion wall portion 94.

Other components of the present invention interact with the various embodiments of the seal in a similar fashion to their interaction with seal 36 of FIG. 2. Prior to use of valve 10, it is preferable that the seal caps 40 or 92 be pierced centrally by a steel needle in the axial direction, precutting the seal to provide the slit 11 in order to allow for more rapid decompression and reformation of the seal upon piercing by the spike 26. The seals are advantageously formed from a material which can repeatedly reseal and prevent fluid from flowing around the seal material. The seal 36 should also be capable of being forced down and then spring back into position to reseal the valve. Material that is too soft will reseal effectively; however, will not be capable of springing back after opening of the valve. Material that is too hard will provide sufficient spring force; however, will not effectively seal. Thus, in a preferred embodiment, the seal is formed from a silicone having a hardness in the range from 30–70 Shore durometer units, and more preferably in the range 40–50 Shore durometer units. A cure silicone polymer in the preferred hardness range is available from Wacker Silicone Corp. of Adrian, Mich. In some embodiments of the invention, it is desirable to provide additional lubricity to the seal 36 to allow it to spring back and reseal more effectively. Dow Chemical Co. produces a silicone formulation with silicone oil built in to provide this additional lubricity.

In general, the closing of the valve 10 is provided not by the side wall of the seal 36 which immediately covers the through-holes 34, but by the seal cap 40, or seal cap 92 filling the proximal end of the cavity 98 and the opening 25a. Thus, the seal caps 40 and 92 are sufficiently thick to reseal the opening 25a effectively after valve closure. However, the seal caps 40 and 92 should also be sufficiently thin to allow them to readily return to the closed position. Preferably the thickness of the caps 40 and 92 ranges between 0.075 and 0.500 inch and more preferably may be approximately 0.100 inch.

The valve disclosed in this invention can be provided in a sterile and disposable form such that after its use in a given installation is exhausted, the device is discarded. However, as described above, in any given installation, the device can be reused multiple times. Since the device does not employ needles, there is little chance that the device will inadvertently cause skin puncture. Therefore, the extra precautions required for handling and disposing of needles is obviated. It will be apparent from the detailed description provided herein that the present invention can provide for the elimination of nearly all needles used in the medical environment. With the use of the valve of the present invention, the need for all needles except those that are directly input into a patient is, advantageously, eliminated.

Operation

The valve 10 is used to provide a closed, patient access system for transferring a predetermined amount of medication from a remote source to the patient. The valve 10 is

US 6,572,592 B1

15

connected by the distal end to the patient, for example, a vein or artery in fluid communication with the valve. Blood fills the valve, but the seal 36d, for example, prevents any blood from leaking from the valve. The delivery end or nose 48 of the medical implement is inserted into the valve as depicted in FIG. 8, pushing the nose 48 against the seal to compress the seal sufficiently to allow the tip 32 of the spike 24 to pierce the seal and enter said delivery end. The predetermined amount of medication in its entirety may now be transferred through the nose 48 into the valve 10 and into the patient. Since the nose 48 and seal 36d engage in a manner so that the tip 32 of the spike element 24, upon piercing the seal, meets the seal to avoid formation of any dead space at the interface between nose 48 and the seal surface 40b. Transfer directly through the valve 10 of essentially the entire predetermined amount of medication from the syringe 46 to the patient, so that essentially none of said predetermined amount is collected in any dead space in the valve, is accomplished with this invention. Upon withdrawing the nose 48 from the valve 10 the seal 36d returns to the decompressed state to close the valve and maintain while in said decompressed state a fluid tight seal even at high pressures and after repeated uses.

Scope of the Invention

The above presents a description of the best mode contemplated of carrying out the present invention, and of the manner and process of making and using it, in such full, clear, concise, and exact terms as to enable any person skilled in the art to which it pertains to make and use this invention. This invention is, however, susceptible to modifications and alternate constructions from that discussed above which are fully equivalent. Consequently, it is not the intention to limit this invention to the particular embodiments disclosed. On the contrary, the intention is to cover all modifications and alternate constructions coming within the spirit and scope of the invention as generally expressed by the following claims, which particularly point out and distinctly claim the subject matter of the invention.

What is claimed is:

1. A medical valve comprising:

a body including an internal cavity having a proximal end and a distal end,

said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end,

a spike have a tip and a passageway with a hole that allows fluid to flow through said passageway, and

a resilient seal which is adapted to be moved into a compressed state upon insertion of the of the medical implement into said opening to open the valve and returns to a decompressed state upon removal of said tip to close said valve,

said seal being pierced by the spike upon being compressed and having a proximal end including a pressure responsive element disposed on an inner surface of the seal adjacent said opening, said pressure responsive element in the decompressed state closing any orifice in the seal at said proximal end to provide an essentially fluid-tight seal while in the decompressed state.

2. The medical valve of claim 1 where said tip has a plurality of facets which meet within a recess.

3. The medical valve of claim 1 where the seal comprises a series of O-ring elements stacked together and connected to form a unitary structure.

4. The medical valve of claim 1 where the pressure responsive element is a section of the seal including an

16

entryway into a precut orifice in the proximal end of the seal, said seal section being surrounded by a space which receives pressurized fluid.

5. The medical valve of claim 1 where the O-ring elements have increasing diameters, with the smallest diameter element being adjacent a proximal end of the seal.

6. The medical valve of claim 1 where there is a cavity in said body having a plurality of radial indentations in an interior wall that is adjacent the seal to accommodate the expansion of the seal upon compression of said seal.

7. The medical valve of claim 1 where the delivery end and the seal are adapted to engage so that when the tip of the spike pierces the seal there is essentially no dead space between said delivery end and the seal.

8. The medical valve of claim 1 where the proximal end of the seal has a centrally located, anti-vacuum, saucer like depression therein, and the pressure responsive element has an anti-tear element.

9. A valve, comprising:

a body having a cavity therein;

a spike located within said cavity in said body; and

a seal located on said spike, said seal comprising a series of O-ring elements.

10. The valve of claim 9, wherein said body includes a connector for connecting to a medical implement and an opening for transmission of fluid between said valve and said medical implement.

11. The valve of claim 10, wherein said spike includes a fluid passageway, an end, and one or more holes for providing fluid communication between said fluid passageway and said medical implement through said one or more holes.

12. The valve of claim 11, wherein said seal has a decompressed position and a compressed position, said seal preventing fluid communication between said fluid passageway and said medical implement when said seal is in said decompressed position and permitting fluid communication between said fluid passageway and said medical implement when said seal is in said compressed position, said seal being compressed to said compressed position when said medical implement is connected to said connector of said body and said seal returning to said decompressed position when said medical implement is disconnected from said connector of said body.

13. The valve of claim 12, wherein said end of said spike is pointed so that it can pierce said seal and enter into a portion of said medical implement when said medical implement is connected to said valve.

14. The valve of claim 13 wherein, fluid flows directly between said medical implement and said spike.

15. The valve of claim 12, wherein said seal is placed over said end of said spike so that said seal covers said end of said spike when said seal is in said decompressed position, but said end of said spike protrudes from said seal when said seal is in said compressed position.

16. The valve of claim 9, wherein the O-ring elements are connected to form a unitary structure.

17. A needleless connector valve comprising:

a body including wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement, the opening being adapted to receive fluid through said delivery end;

a resilient seal which is adapted to be moved distally in the cavity into an axially compressed position upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the

US 6,572,592 B1

17

cavity and returning to an axially uncompressed position upon removal of said delivery end from said opening, said seal in the axially uncompressed position bearing against said wall structure near said opening to seal said opening, said seal having at least one horizontal groove to facilitate movement of said seal between said axially compressed and said axially uncompressed positions, and in the axially compressed position said seal section being located in the cavity distal of said opening, wherein said seal in the uncompressed position has a proximal end substantially flush with the proximal end of said cavity of said body; and

a tube seated in the distal end of said cavity for permitting fluid to flow through the distal end of said cavity, said tube sized such that a portion of said seal fits snugly around the distal end of said tube.

18. The needleless connector valve of claim 17, wherein the distal end of the seal fits snugly within said wall structure.

19. The needleless connector valve of claim 18, wherein said proximal end of said seal is substantially flat.

20. The needleless connector valve of claim 17, wherein said seal moves between said compressed position and said uncompressed position in an accordion-like fashion.

21. The needleless connector valve of claim 17, wherein said seal is precut to form a tiny orifice therein, allowing fluid to pass through said orifice upon compression of said seal in the distal direction.

22. The needleless connector valve of claim 17, wherein the tube is formed integral with surrounding structure.

23. The needleless connector valve of claim 17, wherein said valve further comprises a support member enabling said valve to be removably attached to a fluid dispenser.

24. The needleless connector valve of claim 17, wherein the distal end of said tube is formed integral with surrounding structure.

25. The needleless connector valve of claim 17, wherein said seal comprises an accorded structure.

26. The needleless connector valve of claim 17, wherein said seal comprises a single rubber molding.

27. A valve, comprising:

a body having a cavity therein;

a spike located within said cavity, said spike having a proximal end and at least two holes located distal said proximal end; and

a seal located on said spike, said seal in a decompressed state extending proximal the proximal end of said spike.

28. The valve of claim 27, wherein said seal comprises a series of O-ring elements.

29. The valve of claim 28, wherein the O-ring elements are connected to form a unitary structure.

30. The valve of claim 27, wherein said seal in a compressed state is located distal said at least two holes in said spike.

31. A method of establishing a fluid flow path through a medical connector having an outer housing with a hollow interior and a proximal end and a distal end, comprising:

positioning a tubular seal within said interior, said seal having a proximal end and a distal end and a tubular wall with inner and outer surfaces defining a passage through said seal along an axial centerline extending through said proximal and distal ends, said seal having an axially uncompressed position in which said passage is closed at said seal proximal end, obstructing fluid flow through said connector, at least a portion of said

18

seal near said seal proximal end filling essentially completely a radial cross-section of said housing near said housing proximal end in said uncompressed position, and at least one of said surfaces having alternating radially inwardly and radially outwardly extending surfaces with respect to said centerline while said seal is in the uncompressed position, said seal having an axially compressed position in which said passage is open at said seal proximal end thereof and said passage is unobstructed, said seal having a first axial height H1 when in its uncompressed position and a second axial height H2 when said seal is in its compressed position;

compressing said seal distally within said housing by inserting a medical implement having an end through said proximal end of said housing into said interior of said housing, said end of said medical implement contacting said seal solely at said proximal end of said seal upon insertion of said implement in said interior of said housing;

changing the height of said seal from H1 to H2, where H1 is greater than H2;

opening said passage through said seal along said centerline when said seal is in its compressed position; and establishing fluid flow through said housing from said housing proximal end to said housing distal end thereof.

32. The method of claim 31, wherein said wall comprises a plurality of ring elements, said ring elements having a cross section with a top end and a bottom end and a central portion, said rings joined at their top and bottom ends, and said central portion defining outwardly extending portions.

33. The method of claim 31, wherein said positioning step further comprises the step of positioning said proximal end of said seal flush with said proximal end of said medical connector.

34. The method of claim 31, wherein said seal comprises a single rubber molding.

35. A needleless connector valve comprising:

a body including a wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement, the opening being adapted to receive fluid through said delivery end; and

a seal which is adapted to be moved distally in the cavity into an axially compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to an axially decompressed state upon removal of said medical implement from said opening, said seal substantially completely filling said opening and presenting a generally flush surface across said proximal end of said cavity of said body when said seal is in the decompressed position, said seal having a tubular, corrugated, imperforate wall accommodating axial compression of said seal, and said seal having a preslit orifice at the proximal end of the seal, said orifice being closed to prevent fluid from flowing through said seal when said seal is in said opening, and said orifice being open to allow fluid to flow through said seal when said seal is in the compressed state.

36. The needleless connector valve in accordance with claim 35, wherein said corrugated wall is defined by ring-elements, each of said ring elements having a cross-section with a top end and a bottom end and a central portion, said

US 6,572,592 B1

19

rings joined at their top and bottom ends, and said central portion defining said outwardly extending portions.

37. The needleless connector valve of claim 35, wherein the valve further comprises a tube disposed within said seal near the junction of said seal and the distal end of said cavity, a distal portion of said seal fitting snugly around a portion of said tube.

38. A needleless connector valve comprising:

- a body including an wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end; and
- a seal which is adapted to be moved distally in the cavity into an axially compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to a axially decompressed state upon removal of said medical implement from said opening, said seal substantially completely filling said opening and presenting a generally flush surface across said proximal end of said cavity of said body when said seal is in the decompressed position, said seal having resilient, imperforate bellows accommodating axial compression of said seal, and said seal having a preslit orifice at the proximal end of the seal, said orifice being closed to prevent fluid from flowing through said seal when said seal is in said opening, and said orifice being open to allow fluid to flow through said seal when said seal is in the compressed state.

39. The needleless connector valve of claim 38, wherein the valve further comprises a tube disposed within said seal near the junction of said seal and the distal end of said cavity, a distal portion of said seal fitting snugly around a portion of said tube.

40. The needleless connector valve of claim 38, wherein said seal moves between said compressed state and said decompressed state in an accordion-like fashion.

41. A method of transferring fluid from a remote source to a patient, comprising:

- (a) connecting a medical valve to the patient, wherein the valve comprises a body including wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end, and a resilient seal having a proximal end and a distal end and adapted to be moved distally in the cavity into an axially compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to an axially decompressed state upon removal of said delivery end from said opening, said seal in the decompressed state having a section which fills essentially completely a portion of the cavity adjacent said opening, said seal section bearing against said wall structure near said opening to seal said opening and said seal having a proximal end substantially flush with the proximal end of said cavity of said body, and in the compressed state said seal section being located in the cavity distal said opening, said seal being preslit at the proximal end thereof, and said seal having a plurality of ring elements forming a portion of said seal to facilitate the movement of the seal, said ring elements having a cross-section with a top end and a bottom end and a central portion, said rings joined at their top and bottom ends, and said central portion defining outwardly extending portions;

20

(b) inserting the delivery end of the medical implement into said opening; and

(c) pushing said delivery end into the cavity to compress said seal sufficiently to allow fluid to flow from said medical implement through said valve to the patient.

42. The method of claim 41, wherein said seal comprises a single rubber molding.

43. A medical valve including

- a generally tubular body defining an internal cavity and having a proximal end and a distal end, said proximal end of said body having an opening sufficiently large to receive an ANSI standard tip of a medical implement,
- a hollow spike having a closed tip, said spike including a plurality of holes located inward of said tip, said spike being seated inside the body such that said tip is inward of the proximal end of the body,
- a support member connected to the spike which seals off a portion of the internal cavity of the body such that an upper cavity containing the tip of the spike is defined, and
- a plastic, resilient silicone sealant which fills the upper cavity and covers the tip of the spike so as to present an essentially flush surface.

44. A valve for engaging a medical implement adapted to transfer fluid, comprising:

- a hollow spike having a distal end and a proximal end, said spike having a tip at its proximal end and having at least 3 holes located inward of said tip, said holes being capable of being placed in fluid communication with said medical implement,
- a seal adapted to fit over said spike and to reversibly seal said holes, said seal being adapted to reversibly unseal said holes when said medical implement is engaged with said connector valve; and
- a housing at least partially containing said spike and said seal.

45. A method of transferring a predetermined amount of medication from a remote source to a patient, including

- (a) connecting a medical valve to the patient where the valve includes an opening sufficiently large to receive a delivery end of a medical implement which transfers said predetermined amount of medication through said delivery end into the valve, said valve including an enclosed spike with a tip having a hole therein and a resilient seal which is adapted to be moved into a compressed state by the delivery end upon insertion of said delivery end of the medical implement into said valve and an returns to a decompressed state upon removal of said delivery end to close said valve, said delivery end and said seal being adapted to engage so that the tip of the spike pierces the seal and there is essentially no dead space between said delivery end and the seal;
- (b) inserting the delivery end of the medical implement into said valve and pushing said delivery end against said seal to compress said seal sufficiently to allow said tip of the spike to pierce the seal and enter said delivery end, said seal and delivery end engaging to eliminate essentially any dead space;
- (c) transferring from the remote source to the patient directly through said valve essentially the entire predetermined amount of medication, so that essentially none of said predetermined amount is collected in any dead space in the valve; and
- (d) withdrawing the delivery end of the medical implement from the valve to enable the seal to return to the

US 6,572,592 B1

21

decompressed state to close the valve and maintain while in said decompressed state a fluid tight seal even at high pressures and repeated uses.

46. A method of transferring fluid from a remote source to a patient, comprising:

- (a) connecting a medical valve to the patient, wherein the valve comprises a body including wall structure defining an internal cavity having a proximal end and a distal end, said proximal end having an opening sufficiently large to receive a delivery end of a medical implement which transfers fluid through said delivery end, a resilient seal having a proximal end and a distal end and adapted to be moved distally in the cavity into an axially compressed state upon insertion of the delivery end of the medical implement into said opening, said seal moving proximally in the cavity and returning to an axially decompressed state upon removal of said delivery end from said opening, said seal in the decompressed state having a section which fills essentially completely a portion of the cavity adjacent said open-

22

ing and presenting a generally flush surface across said proximal end of said cavity of said body, and in the compressed state said seal section being located in the cavity distal said opening, said seal being pre-slit at the proximal end thereof, wherein said seal has at least one horizontal groove to facilitate the movement of the seal, and a tube disposed within said seal near the junction of said seal and the distal end of the cavity, the tube sized such that a portion of said seal fits snugly around a portion of the tube near the distal end of the cavity;

- (b) inserting the delivery end of the medical implement into said opening; and
- (c) pushing said delivery end into the cavity to axially compress said seal sufficiently to allow fluid to flow from said medical implement through said valve to the patient.

* * * * *

JS 44 (Rev. 3/99)

CIVIL COVER SHEET

The JS-44 civil cover sheet and the information contained herein neither replace nor supplement the filing and service of pleadings or other papers as required by law, except as provided by local rules of court. This form, approved by the Judicial Conference of the United States in September 1974, is required for the use of the Clerk of Court for the purpose of initiating the civil docket sheet. (SEE INSTRUCTIONS ON THE REVERSE OF THE FORM.)

I. (a) PLAINTIFFS

ICU MEDICAL, INC.

DEFENDANTS

RYMED TECHNOLOGIES, INC.

(b) County of Residence of First Listed Plaintiff _____
(EXCEPT IN U.S. PLAINTIFF CASES)

County of Residence of First Listed Defendant _____
(IN U.S. PLAINTIFF CASES ONLY)

NOTE: IN LAND CONDEMNATION CASES, USE THE LOCATION OF THE LAND INVOLVED.

(c) Attorney's (Firm Name, Address, and Telephone Number)

Richard L. Horwitz (#2246)
Potter Anderson & Corroon LLP
1313 N. Market Street
Wilmington, Delaware 19801 (302) 984-6000

Attorneys (If Known)

II. BASIS OF JURISDICTION (Place an "X" in One Box Only)

- ☐ 1 U.S. Government Plaintiff ☒ 3 Federal Question (U.S. Government Not a Party)
- ☐ 2 U.S. Government Defendant ☐ 4 Diversity (Indicate Citizenship of Parties in Item III)

III. CITIZENSHIP OF PRINCIPAL PARTIES (Place an "X" in One Box for Plaintiff and One Box for Defendant)

(For Diversity Cases Only)

- Citizen of This State PTF ☐ 1 DEF ☐ 1 Incorporated or Principal Place of Business In This State PTF ☐ 4 DEF ☐ 4
- Citizen of Another State ☐ 2 ☐ 2 Incorporated and Principal Place of Business In Another State ☐ 5 ☐ 5
- Citizen or Subject of a Foreign Country ☐ 3 ☐ 3 Foreign Nation ☐ 6 ☐ 6

IV. NATURE OF SUIT (Place an "X" in One Box Only)

CONTRACT	TORTS	FORFEITURE/PENALTY	BANKRUPTCY	OTHER STATUTES
<input type="checkbox"/> 110 Insurance <input type="checkbox"/> 120 Marine <input type="checkbox"/> 130 Miller Act <input type="checkbox"/> 140 Negotiable Instrument <input type="checkbox"/> 150 Recovery of Overpayment & Enforcement of Judgment <input type="checkbox"/> 151 Medicare Act <input type="checkbox"/> 152 Recovery of Defaulted Student Loans (Excl. Veterans) <input type="checkbox"/> 153 Recovery of Overpayment of Veteran's Benefits <input type="checkbox"/> 160 Stockholders' Suits <input type="checkbox"/> 190 Other Contract <input type="checkbox"/> 195 Contract Product Liability	PERSONAL INJURY <input type="checkbox"/> 310 Airplane <input type="checkbox"/> 315 Airplane Product Liability <input type="checkbox"/> 320 Assault, Libel & Slander <input type="checkbox"/> 330 Federal Employers' Liability <input type="checkbox"/> 340 Marine <input type="checkbox"/> 345 Marine Product Liability <input type="checkbox"/> 350 Motor Vehicle <input type="checkbox"/> 355 Motor Vehicle Product Liability <input type="checkbox"/> 360 Other Personal Injury	<input type="checkbox"/> 362 Personal Injury—Med. Malpractice <input type="checkbox"/> 365 Personal Injury—Product Liability <input type="checkbox"/> 368 Asbestos Personal Injury Product Liability PERSONAL PROPERTY <input type="checkbox"/> 370 Other Fraud <input type="checkbox"/> 371 Truth in Lending <input type="checkbox"/> 380 Other Personal Property Damage <input type="checkbox"/> 385 Property Damage Product Liability	<input type="checkbox"/> 422 Appeal 28 USC 158 <input type="checkbox"/> 423 Withdrawal 28 USC 157 PROPERTY RIGHTS <input type="checkbox"/> 820 Copyrights <input checked="" type="checkbox"/> 830 Patent <input type="checkbox"/> 840 Trademark	<input type="checkbox"/> 400 State Reapportionment <input type="checkbox"/> 410 Antitrust <input type="checkbox"/> 430 Banks and Banking <input type="checkbox"/> 450 Commerce/ICC Rates/etc. <input type="checkbox"/> 460 Deportation <input type="checkbox"/> 470 Racketeer Influenced and Corrupt Organizations <input type="checkbox"/> 810 Selective Service <input type="checkbox"/> 850 Securities/Commodities/Exchange <input type="checkbox"/> 875 Customer Challenge 12 USC 3410 <input type="checkbox"/> 891 Agricultural Acts <input type="checkbox"/> 892 Economic Stabilization Act <input type="checkbox"/> 893 Environmental Matters <input type="checkbox"/> 894 Energy Allocation Act <input type="checkbox"/> 895 Freedom of Information Act <input type="checkbox"/> 900 Appeal of Fee Determination Under Equal Access to Justice <input type="checkbox"/> 950 Constitutionality of State Statutes <input type="checkbox"/> 890 Other Statutory Actions
REAL PROPERTY <input type="checkbox"/> 210 Land Condemnation <input type="checkbox"/> 220 Foreclosure <input type="checkbox"/> 230 Rent Lease & Ejectment <input type="checkbox"/> 240 Torts to Land <input type="checkbox"/> 245 Tort Product Liability <input type="checkbox"/> 290 All Other Real Property	CIVIL RIGHTS <input type="checkbox"/> 441 Voting <input type="checkbox"/> 442 Employment <input type="checkbox"/> 443 Housing/Accommodations <input type="checkbox"/> 444 Welfare <input type="checkbox"/> 440 Other Civil Rights	PRISONER PETITIONS <input type="checkbox"/> 510 Motions to Vacate Sentence <input type="checkbox"/> Habeas Corpus: <input type="checkbox"/> 530 General <input type="checkbox"/> 535 Death Penalty <input type="checkbox"/> 540 Mandamus & Other <input type="checkbox"/> 550 Civil Rights <input type="checkbox"/> 555 Prison Condition	<input type="checkbox"/> 610 Agriculture <input type="checkbox"/> 620 Other Food & Drug <input type="checkbox"/> 625 Drug Related Seizure of Property 21 USC <input type="checkbox"/> 630 Liquor Laws <input type="checkbox"/> 640 R.R. & Truck <input type="checkbox"/> 650 Airline Regs. <input type="checkbox"/> 660 Occupational Safety/Health <input type="checkbox"/> 690 Other LABOR <input type="checkbox"/> 710 Fair Labor Standards Act <input type="checkbox"/> 720 Labor/Mgmt. Relations <input type="checkbox"/> 730 Labor/Mgmt. Reporting & Disclosure Act <input type="checkbox"/> 740 Railway Labor Act <input type="checkbox"/> 790 Other Labor Litigation <input type="checkbox"/> 791 Empl. Ret. Inc. Security Act	<input type="checkbox"/> 861 HIA (1395ff) <input type="checkbox"/> 862 Black Lung (923) <input type="checkbox"/> 863 DIWC/DIWW (405(g)) <input type="checkbox"/> 864 SSID Title XVI <input type="checkbox"/> 865 RSI (405(g)) FEDERAL TAX SUITS <input type="checkbox"/> 870 Taxes (U.S. Plaintiff or Defendant) <input type="checkbox"/> 871 IRS—Third Party 26 USC 7609

V. ORIGIN

(PLACE AN "X" IN ONE BOX ONLY)

- ☒ 1 Original Proceeding ☐ 2 Removed from State Court ☐ 3 Remanded from Appellate Court ☐ 4 Reinstated or Reopened ☐ 5 Transferred from another district (specify) ☐ 6 Multidistrict Litigation ☐ 7 Appeal to District Judge from Magistrate Judgment

VI. CAUSE OF ACTION

(Cite the U.S. Civil Statute under which you are filing and write brief statement of cause.
Do not cite jurisdictional statutes unless diversity.)

35 U.S.C § 271 for patent infringement and 28 U.S.C. § 1338(a).

VII. REQUESTED IN COMPLAINT:

☐ CHECK IF THIS IS A CLASS ACTION UNDER F.R.C.P. 23

DEMAND \$

CHECK YES only if demanded in complaint:

JURY DEMAND: ☒ Yes ☐ No**VIII. RELATED CASE(S) IF ANY**

(See instructions):

JUDGE

DOCKET NUMBER

DATE
07/27/2007

SIGNATURE OF ATTORNEY OF RECORD

FOR OFFICE USE ONLY

RECEIPT # _____ AMOUNT _____ APPLYING IFP _____ JUDGE _____ MAG. JUDGE _____

AO FORM 85 RECEIPT (REV. 9/04)

United States District Court for the District of Delaware

07 - 468

Civil Action No. _____

ACKNOWLEDGMENT
OF RECEIPT FOR AO FORM 85

NOTICE OF AVAILABILITY OF A
UNITED STATES MAGISTRATE JUDGE
TO EXERCISE JURISDICTION

I HEREBY ACKNOWLEDGE RECEIPT OF 2 COPIES OF AO FORM 85.

7/27/07

(Date forms issued)

x Mike Bobish

(Signature of Party or their Representative)

x Mike Bobish

(Printed name of Party or their Representative)

Note: Completed receipt will be filed in the Civil Action